

Sample Name :Iα52  
 Cat. No. : RP20228  
 Lot. No. :E7047519J  
 Time Processed :9:06:23  
 Month-Day-Year Processed :10/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

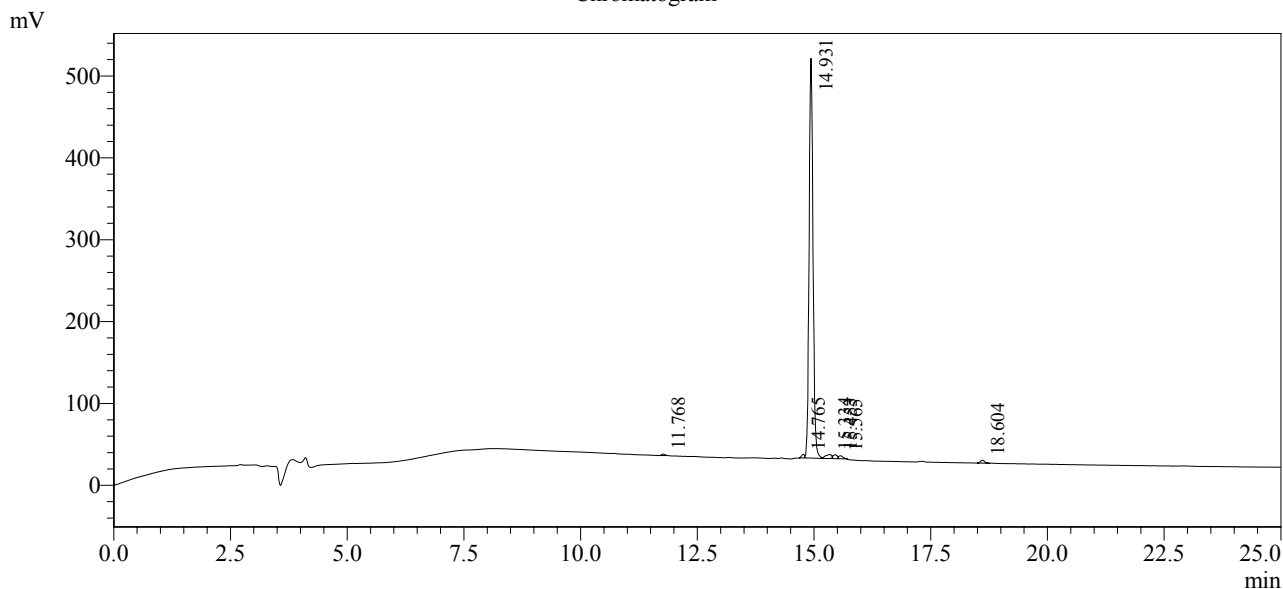

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.768	8736	1806	0.291
2	14.765	19012	4275	0.633
3	14.931	2858164	488493	95.224
4	15.334	44743	4978	1.491
5	15.453	28617	4738	0.953
6	15.565	21696	3612	0.723
7	18.604	20541	3557	0.684
Total		3001509	511460	100.000