

Sample Name :Angiotensin II (3-8), human
 Cat No :RP11253
 Lot No :E8717720J
 Time Processed :18:28:48
 Month-Day-Year Processed :10/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

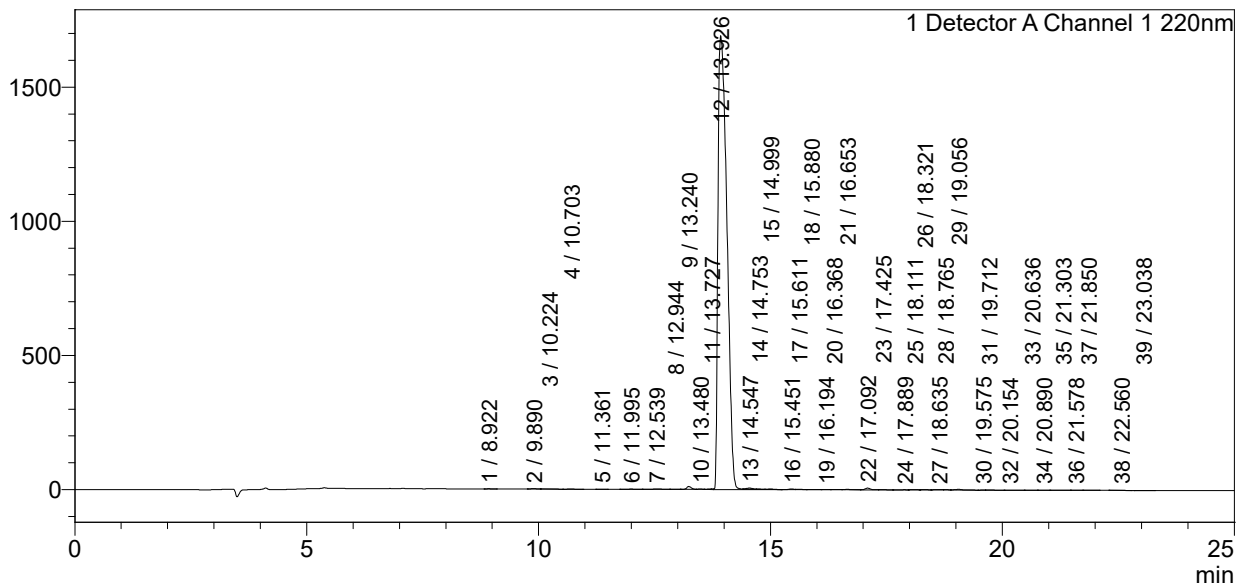

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.922	4585	765	0.020
2	9.890	14566	2107	0.063
3	10.224	10142	992	0.044
4	10.703	7644	867	0.033
5	11.361	1818	240	0.008
6	11.995	12315	1002	0.053
7	12.539	22210	1432	0.096
8	12.944	2260	316	0.010
9	13.240	77260	10790	0.334
10	13.480	12112	1610	0.052
11	13.727	20867	2479	0.090
12	13.926	22653287	1691709	97.852
13	14.547	36030	3849	0.156
14	14.753	5417	895	0.023
15	14.999	14743	1458	0.064
16	15.451	19065	2597	0.082

Peak#	Ret. Time	Area	Height	Area%
17	15.611	9743	1182	0.042
18	15.880	4582	438	0.020
19	16.194	4725	726	0.020
20	16.368	3383	470	0.015
21	16.653	15301	1381	0.066
22	17.092	50451	6260	0.218
23	17.425	7310	760	0.032
24	17.889	6092	586	0.026
25	18.111	16211	1782	0.070
26	18.321	15376	1751	0.066
27	18.635	22920	1809	0.099
28	18.765	10168	1363	0.044
29	19.056	30215	2495	0.131
30	19.575	1466	195	0.006
31	19.712	4755	359	0.021
32	20.154	4280	280	0.018
33	20.636	2464	208	0.011
34	20.890	5477	692	0.024
35	21.303	8558	719	0.037
36	21.578	1582	233	0.007
37	21.850	1672	157	0.007
38	22.560	5396	340	0.023
39	23.038	4179	300	0.018
Total		23150626	1747595	100.000