

Sample Name:Hepatitis B Virus Core (128-140)

Cat. No. : RP17313

Lot. No. : E5589119J

Time Processed: 2:47:30

Month-Day-Year Processed :10/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Equipment:ZJ19010324

<Chromatogram>

mV

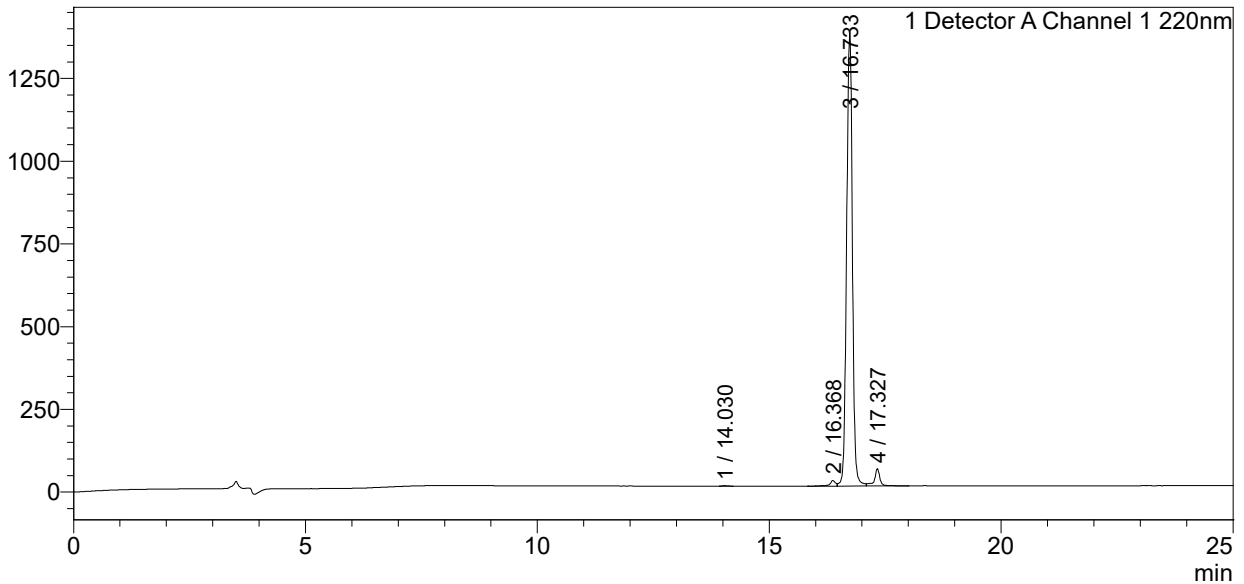

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.030	8574	1381	0.069
2	16.368	147476	16767	1.180
3	16.733	11906556	1368719	95.255
4	17.327	437120	52340	3.497
Total		12499727	1439206	100.000