

Sample Information

Sample Name : Fibronectin Active Fragment Control
 Cat. No. : RP20347
 Lot. No. : PE6571712

Pump A : 0.065% trifluoroacetic in 100% waters (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)


<<Pump>>
 Flow : 1.0000 mL/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	0	
5.00	Pumps	Solvent B Conc.	0	
20.00	Pumps	Solvent B Conc.	30	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
31.00	Pumps	Solvent B Conc.	95	
31.01	Pumps	Solvent B Conc.	0	
40.00	Pumps	Solvent B Conc.	0	
40.01	Controller	Stop		

<<Column Performance>>
 <Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm

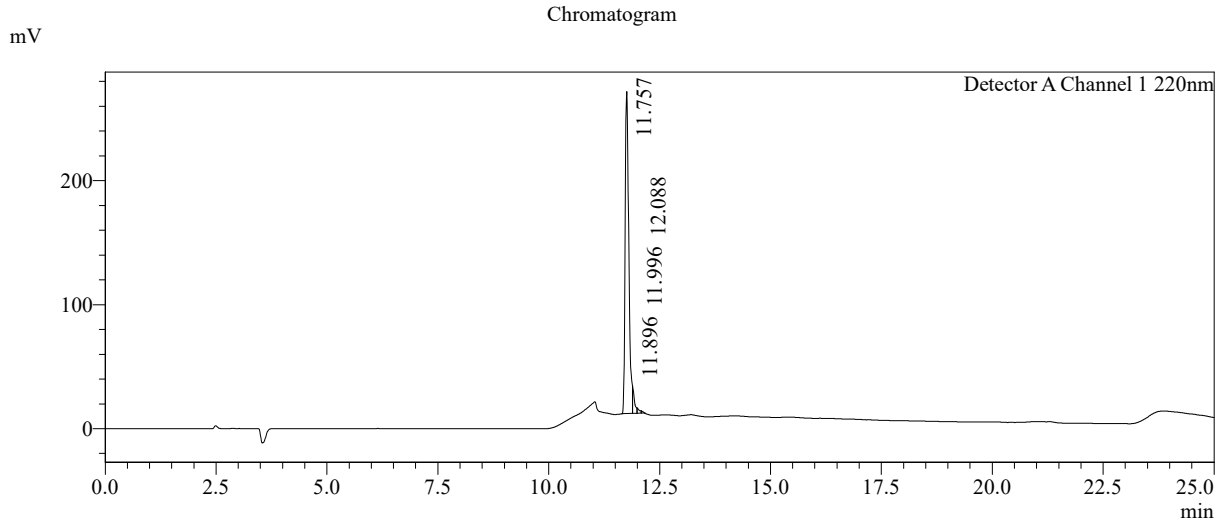

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Height	Area	Height%	Area%
1	11.757	259535	1480388	90.288	95.200
2	11.896	21902	56546	7.619	3.636
3	11.996	4239	14008	1.475	0.901
4	12.088	1777	4079	0.618	0.262
Total		287453	1555021	100.000	100.000