

Sample Name : N-Boc-Phe-Leu-Phe-Leu-Phe
 Cat. No. : RP12950
 Lot. No. : E4472819K
 Time Processed : 8:49:40
 Month-Day-Year Processed : 12/05/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

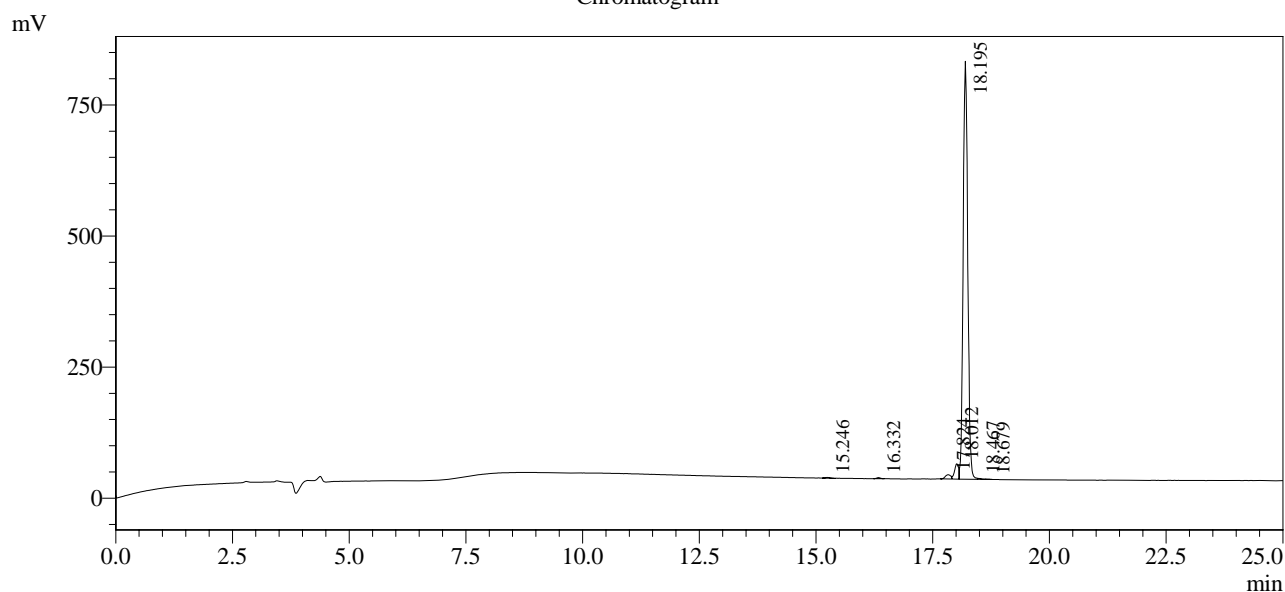

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.246	9323	1460	0.162
2	16.332	12189	2125	0.212
3	17.824	66452	8052	1.155
4	18.012	179347	29198	3.116
5	18.195	5474285	797130	95.117
6	18.467	10481	1968	0.182
7	18.679	3213	482	0.056
Total		5755290	840415	100.000