

Sample Name :Cortistatin 14, human, rat  
 Cat No. : RP10972  
 Lot No. : PE6041901  
 Time Processed : 9:13:12  
 Month-Day-Year Processed : 01/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

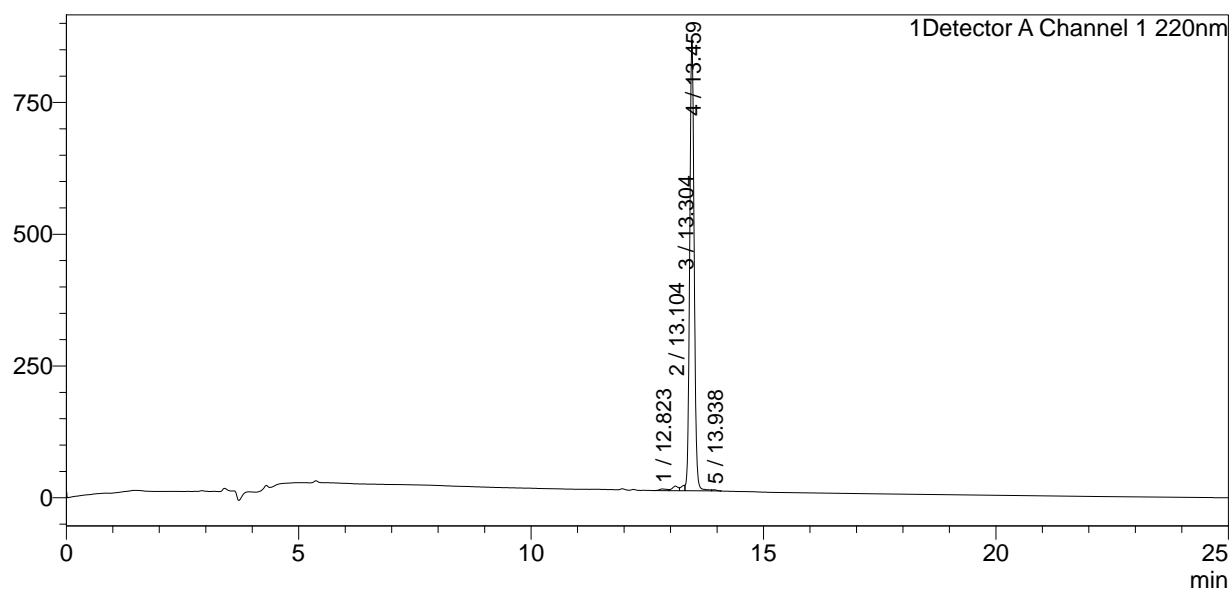

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.823	36086	3108	0.613
2	13.104	77120	8658	1.310
3	13.304	58403	10025	0.992
4	13.459	5698819	854293	96.832
5	13.938	14846	2154	0.252
Total		5885275	878238	100.000