


Mass Spectrum

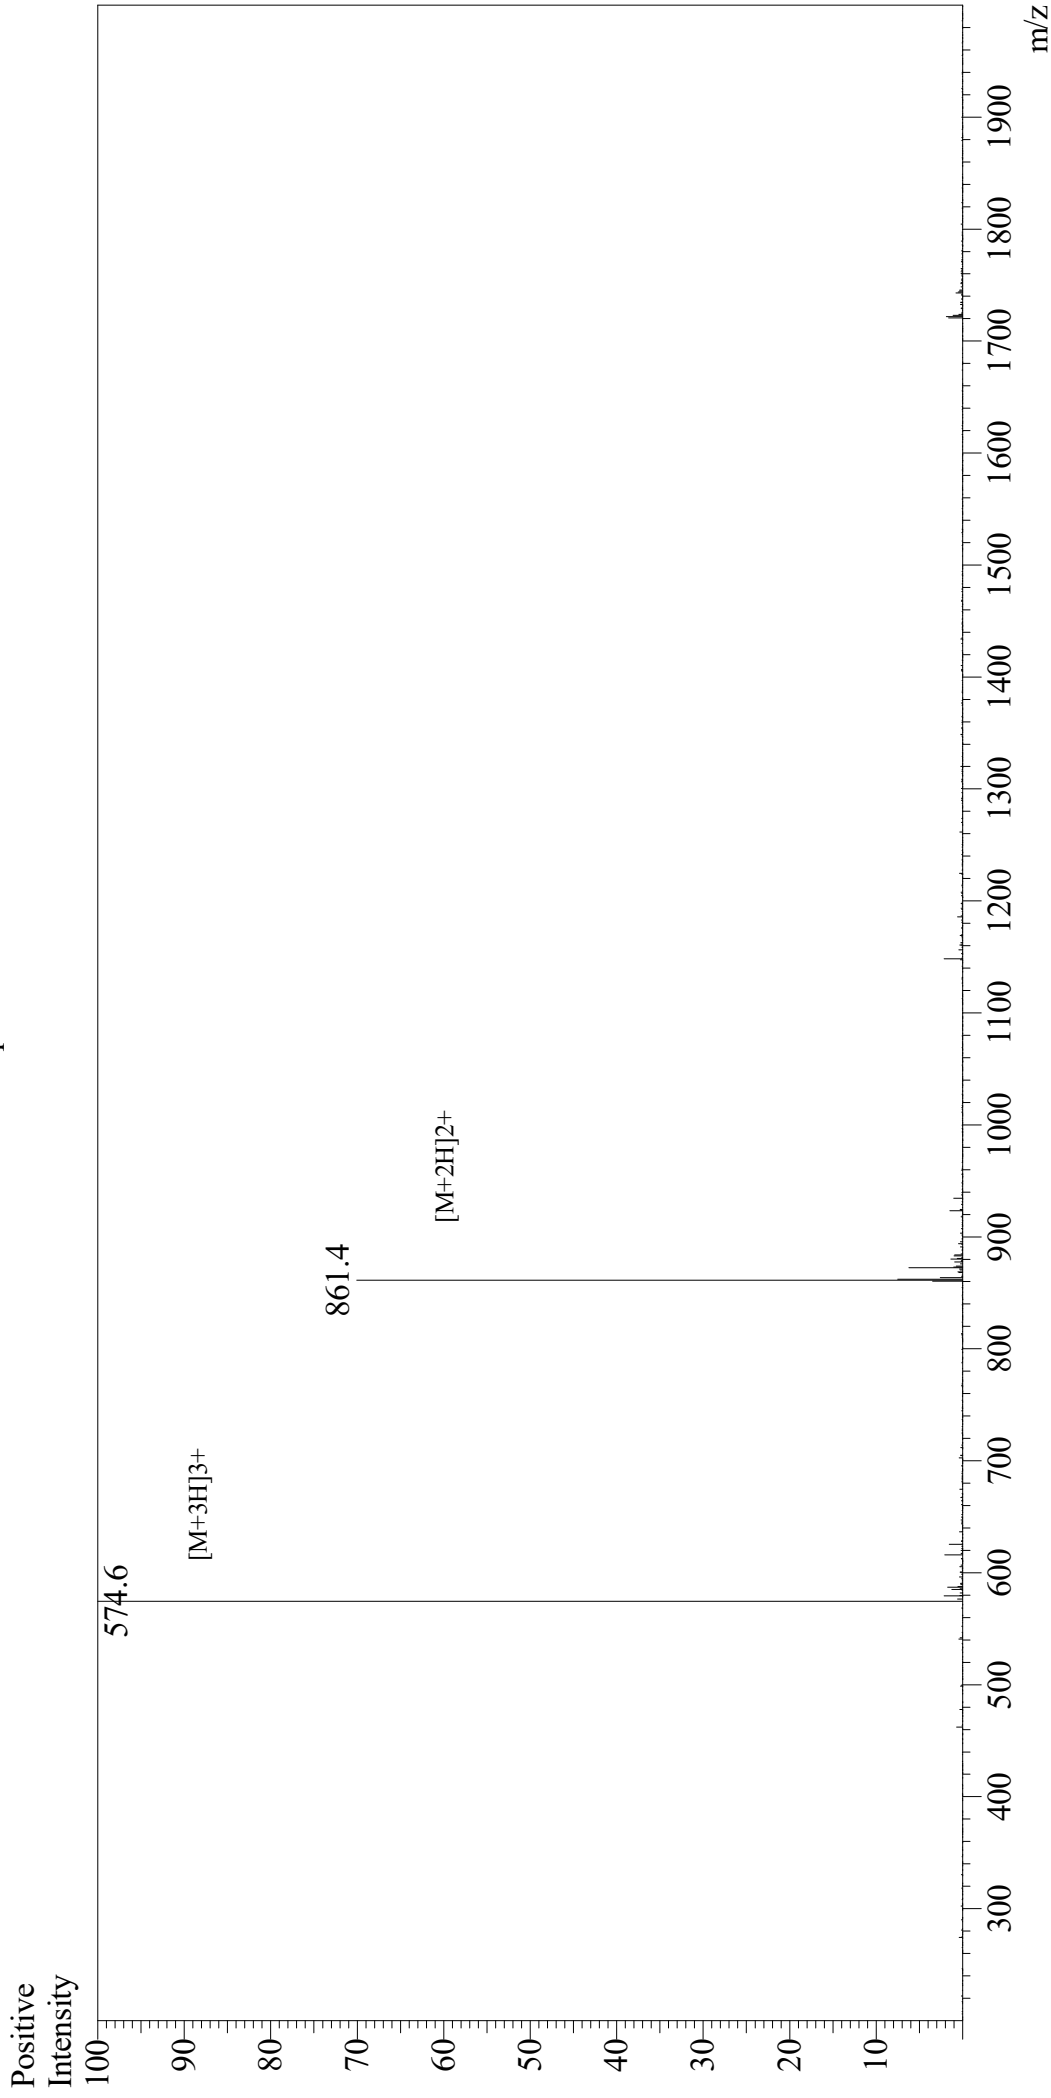

Sample Information

User : Gary
Month-Day Processed : 01/03/19
Time Processed : 07:35:07 PM
Injection Volume : 0.2
Sample Name : Cortistatin 14, human, rat
Cat No. : RP10972
Lot No. : PE6041901
Theoretical MW : 1721.01
Observed MW : 1720.8

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH