

Sample Name : Physalaemin
 Cat. No. : RP10474
 Lot. No. : PE4641808

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

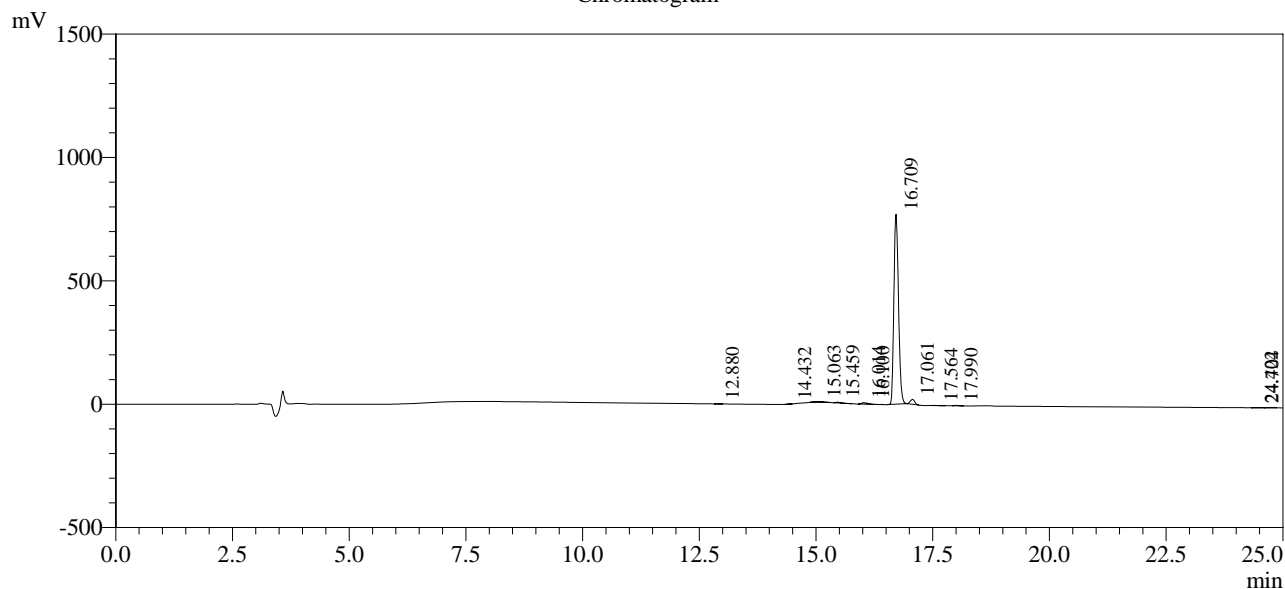

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.880	1163	243	0.021
2	14.432	4216	682	0.076
3	15.063	41154	2864	0.739
4	15.459	20894	2870	0.375
5	16.014	43429	6093	0.779
6	16.100	17117	4243	0.307
7	16.709	5294818	770046	95.033
8	17.061	129086	19832	2.317
9	17.564	5129	871	0.092
10	17.990	8905	1545	0.160
11	24.422	3459	498	0.062
12	24.704	2215	330	0.040
Total		5571585	810117	100.000