

Sample Name:sgp91 ds-tat Peptide 2, scrambled
 Cat. No. : RP20436
 Lot. No. : E3644720A
 Time Processed : 13:44:48
 Month-DaY-Year Processed : 01/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
30.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

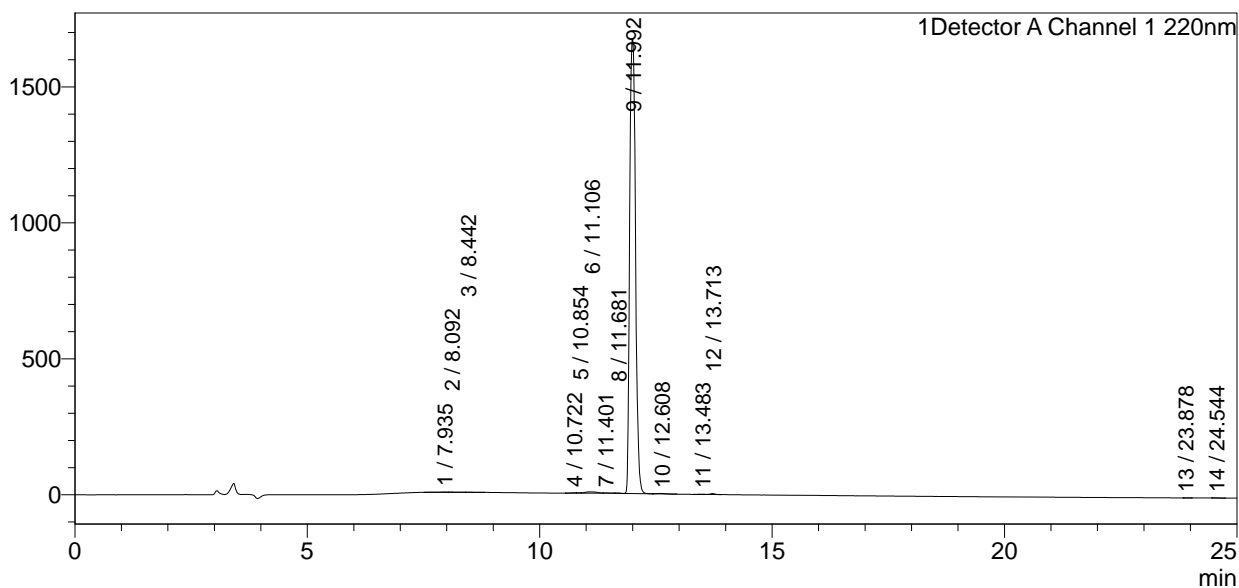

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.935	18876	889	0.128
2	8.092	18282	915	0.124
3	8.442	7575	592	0.051
4	10.722	10705	1344	0.073
5	10.854	7555	1328	0.051
6	11.106	88027	4872	0.598
7	11.401	7466	851	0.051
8	11.681	4765	932	0.032
9	11.992	14497046	1673056	98.517
10	12.608	25671	2109	0.174
11	13.483	6013	744	0.041
12	13.713	20764	3198	0.141
13	23.878	1088	153	0.007
14	24.544	1379	122	0.009
Total		14715213	1691106	100.000