

Sample Name :Fibronectin Active Fragment Control  
 Cat No :RP20347  
 Lot No :E8090721C  
 Time Processed :14:44:02  
 Month-Day-Year Processed :03/20/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
95.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

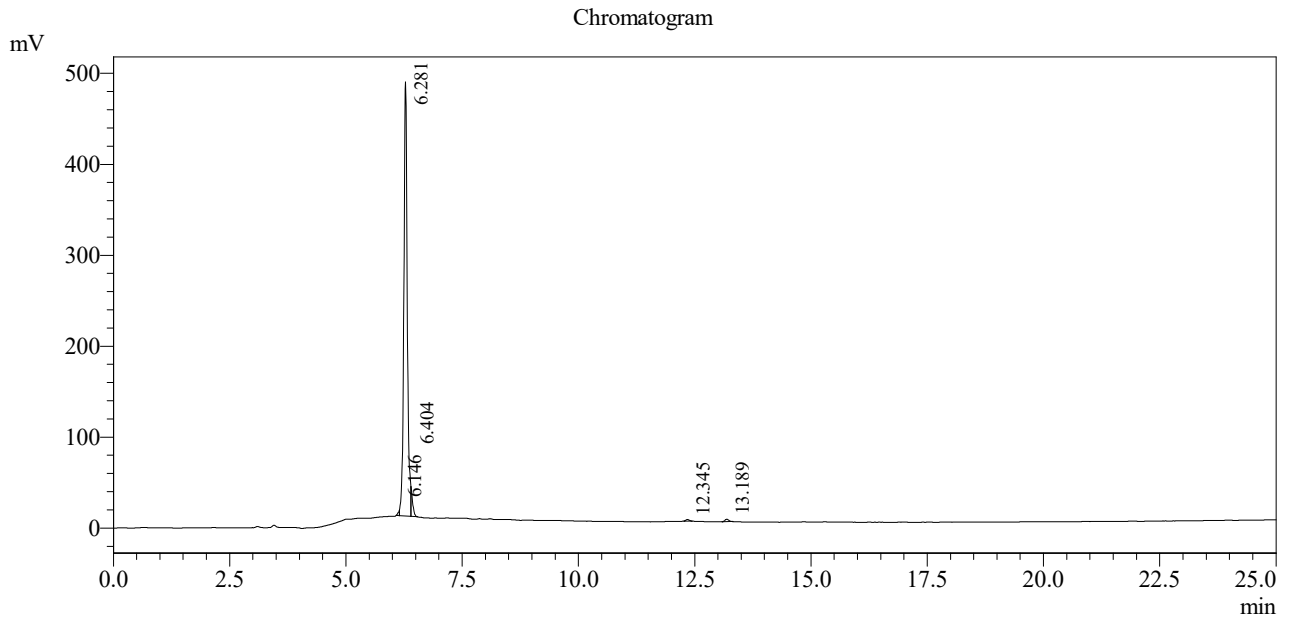

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	6.146	12061	4684	0.465
2	6.281	2493237	477397	96.072
3	6.404	66283	32727	2.554
4	12.345	8172	1634	0.315
5	13.189	15409	2699	0.594
Total		2595162	519140	100.000