

Sample Name : γ -1-Melanocyte Stimulating Hormone (MSH), amide
 Cat No. : RP10650
 Lot No. : PE2471905
 Time Processed : 9:28:14
 Month-Day-Year Processed : 06/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

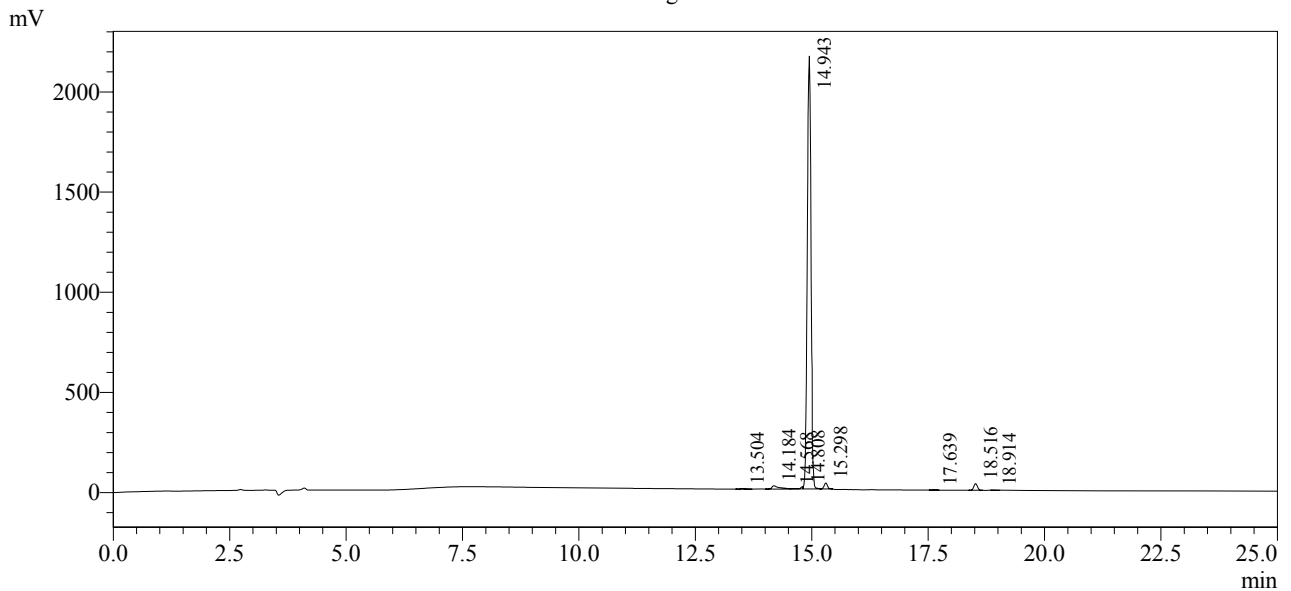

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.504	14273	2606	0.112
2	14.184	190686	16547	1.500
3	14.568	13073	2020	0.103
4	14.808	44593	12086	0.351
5	14.943	12116250	2159948	95.296
6	15.298	142208	29662	1.118
7	17.639	6512	1315	0.051
8	18.516	179366	33080	1.411
9	18.914	7393	1495	0.058
Total		12714356	2258760	100.000