

Sample Name :mTRP-2(180-188)
 Cat No. :RP20250
 Lot No. :E7534919K
 Time Processed :7:49:49
 Month-Day-Year Processed :11/09/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

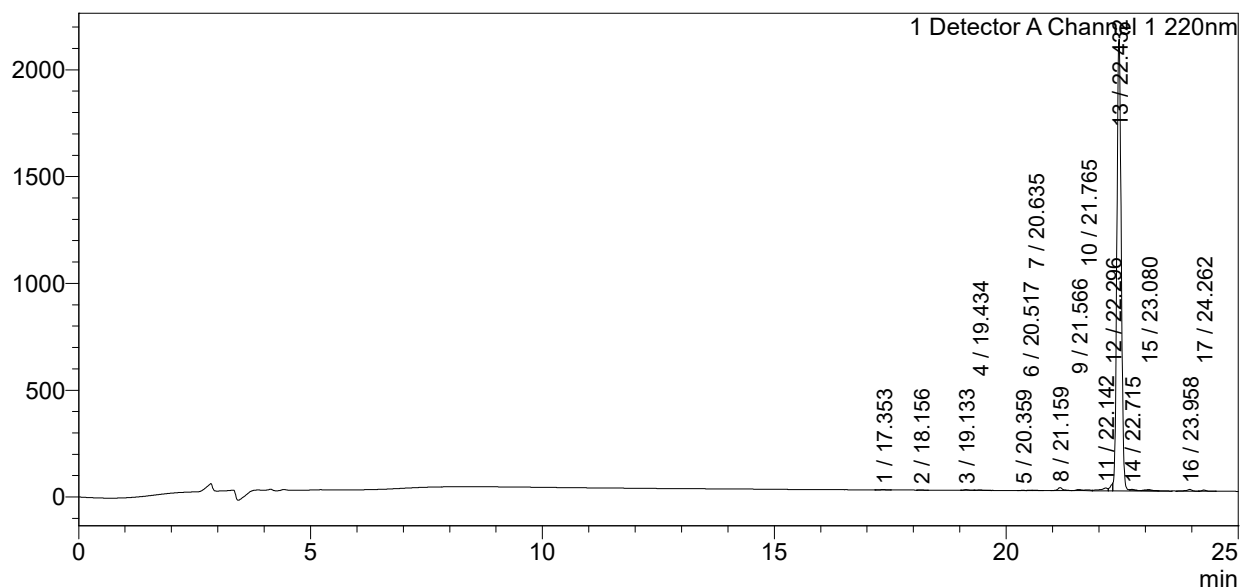

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.353	10687	1181	0.073
2	18.156	3791	571	0.026
3	19.133	19288	3052	0.132
4	19.434	17338	2432	0.118
5	20.359	4547	736	0.031
6	20.517	5840	833	0.040
7	20.635	11610	1818	0.079
8	21.159	111379	14147	0.760
9	21.566	50422	5786	0.344
10	21.765	37637	4513	0.257
11	22.142	138671	13145	0.946
12	22.296	132586	32781	0.905
13	22.432	13958107	2115128	95.255
14	22.715	12324	2738	0.084
15	23.080	42228	4592	0.288

Peak#	Ret. Time	Area	Height	Area%
16	23.958	62204	7946	0.425
17	24.262	34712	5514	0.237
Total		14653372	2216913	100.000