

Sample Name : Osteogenic Growth Peptide, OGP
 Cat. No. : RP20311
 Lot. No. : PE1921903
 Time Processed : 15:09:50
 Month-Day-Year Processed : 03/14/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

Chromatogram

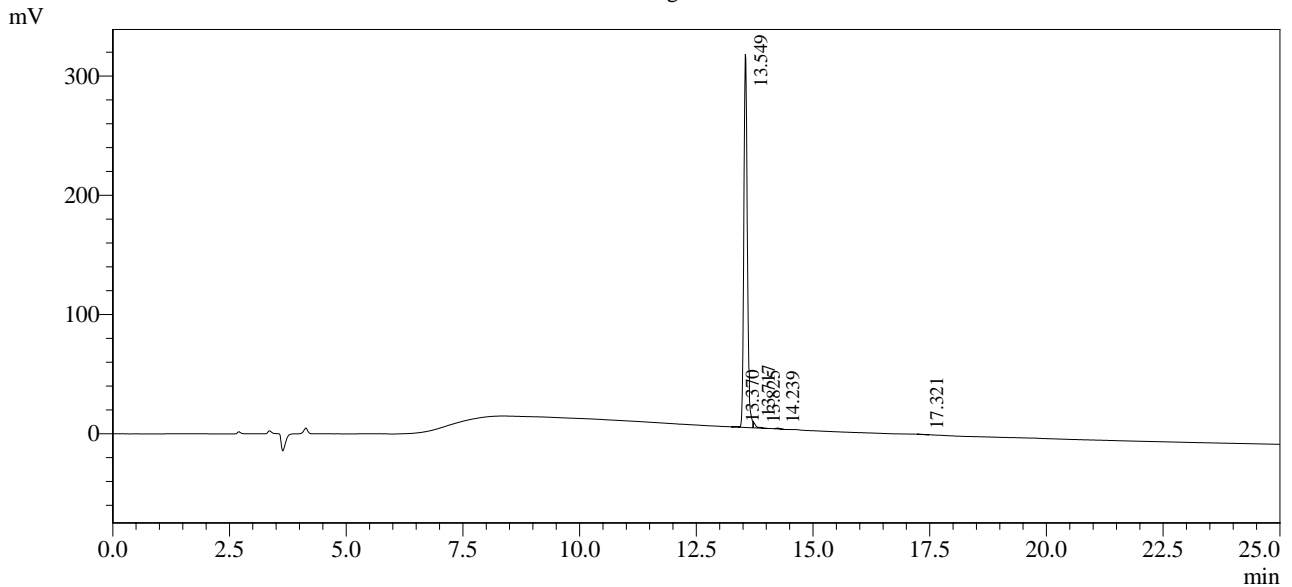

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.370	2239	384	0.134
2	13.549	1644385	312926	98.490
3	13.717	14009	5213	0.839
4	13.825	3655	514	0.219
5	14.239	3283	682	0.197
6	17.321	2021	351	0.121
Total		1669593	320070	100.000