

Sample Name : Neuropeptide Y, human
 Cat. No. : RP10492
 Lot. No. : PE3421901
 Time Processed : 21:23:46
 Month-Day-Year Processed : 01/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
10.00	Pumps	Pump A B.Conc	35	
35.00	Pumps	Pump A B.Conc	95	
41.00	Pumps	Pump A B.Conc	95	
41.01	Pumps	Pump A B.Conc	5	
50.00	Pumps	Pump A B.Conc	5	
50.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

Chromatogram

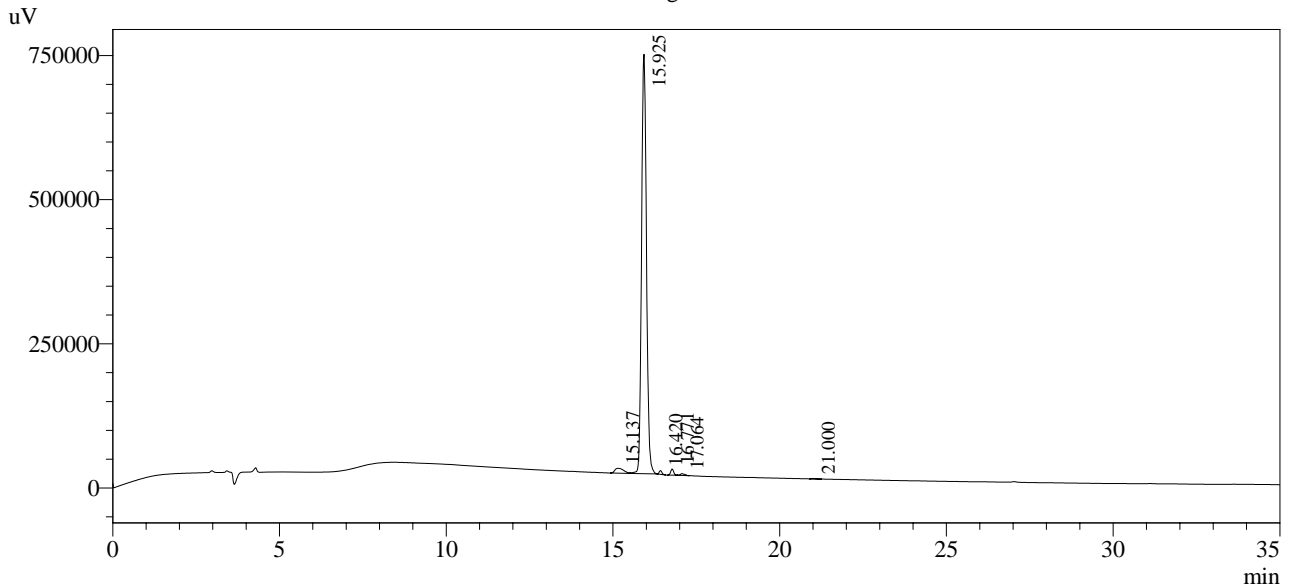

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.137	154186	8291	1.996
2	15.925	7438271	727320	96.315
3	16.420	36633	6471	0.474
4	16.771	64438	10592	0.834
5	17.064	26487	3016	0.343
6	21.000	2878	359	0.037
Total		7722892	756049	100.000