

Sample Name :  $\beta$ -Amyloid (25-35)  
 Cat. No. : RP10008  
 Lot. No. : PE4181612

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima<sup>TM</sup> C18 4.6 x 250 mm

Chromatogram

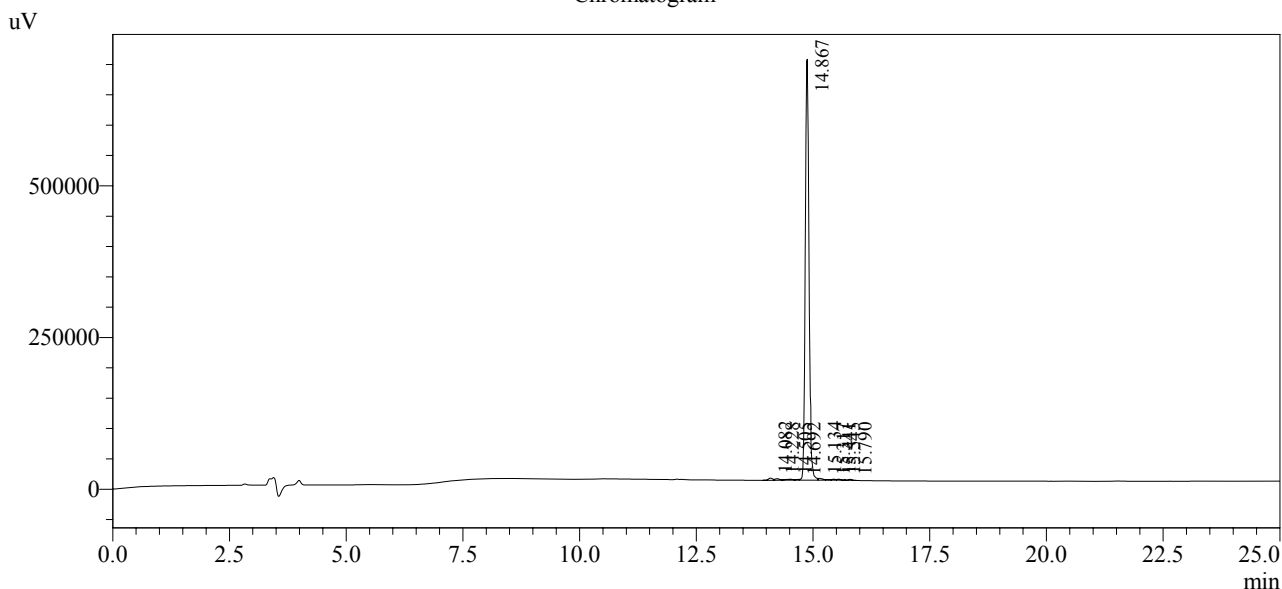

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.082	22701	3545	0.573
2	14.228	18231	2622	0.460
3	14.505	19260	1578	0.486
4	14.692	6107	1302	0.154
5	14.867	3844560	693874	97.052
6	15.134	19394	2852	0.490
7	15.317	6349	919	0.160
8	15.441	7993	1453	0.202
9	15.545	8315	1539	0.210
10	15.790	8429	1536	0.213
Total		3961338	711218	100.000