

Sample Name :Oxytocin
 Cat. No. : RP10407
 Lot. No. : E9385821D
 Time Processed :6:37:30
 Month-Day-Year Processed :05/07/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ20010139

<Chromatogram>

mV

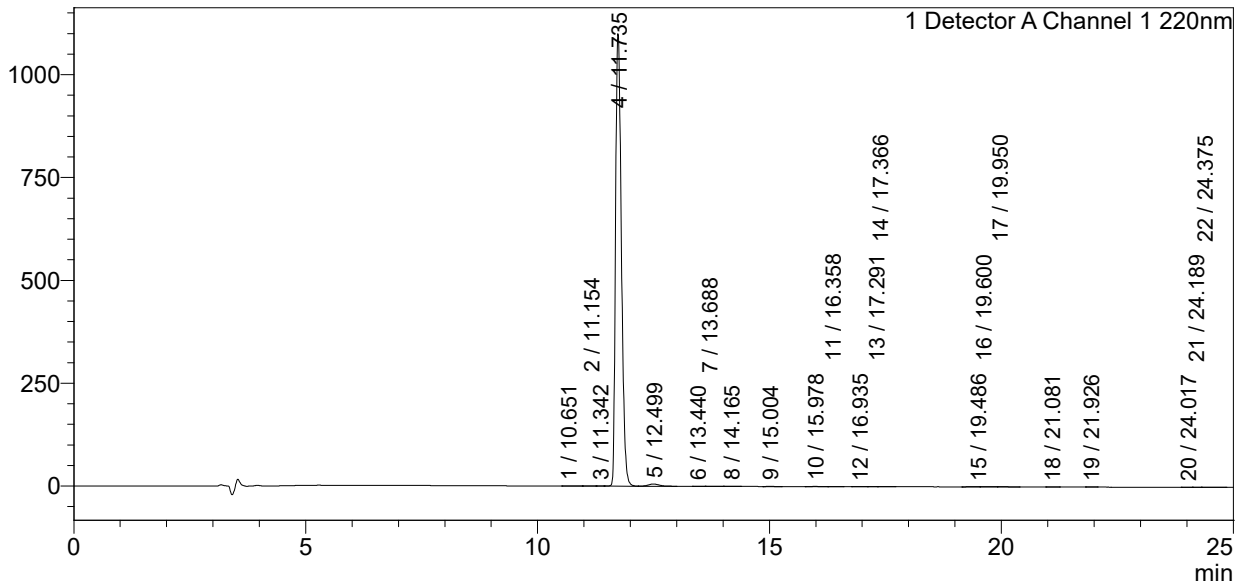

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.651	1371	106	0.014
2	11.154	3208	375	0.033
3	11.342	2619	282	0.027
4	11.735	9637210	1100270	98.483
5	12.499	94123	5413	0.962
6	13.440	2101	197	0.021
7	13.688	1767	133	0.018
8	14.165	1264	117	0.013
9	15.004	1847	231	0.019
10	15.978	3264	327	0.033
11	16.358	1090	131	0.011
12	16.935	1333	133	0.014
13	17.291	1533	202	0.016
14	17.366	2417	210	0.025
15	19.486	8433	586	0.086
16	19.600	10265	585	0.105

Peak#	Ret. Time	Area	Height	Area%
17	19.950	3576	304	0.037
18	21.081	1741	203	0.018
19	21.926	1034	114	0.011
20	24.017	1955	216	0.020
21	24.189	1893	201	0.019
22	24.375	1658	153	0.017
Total		9785701	1110489	100.000