


# Mass Spectrum

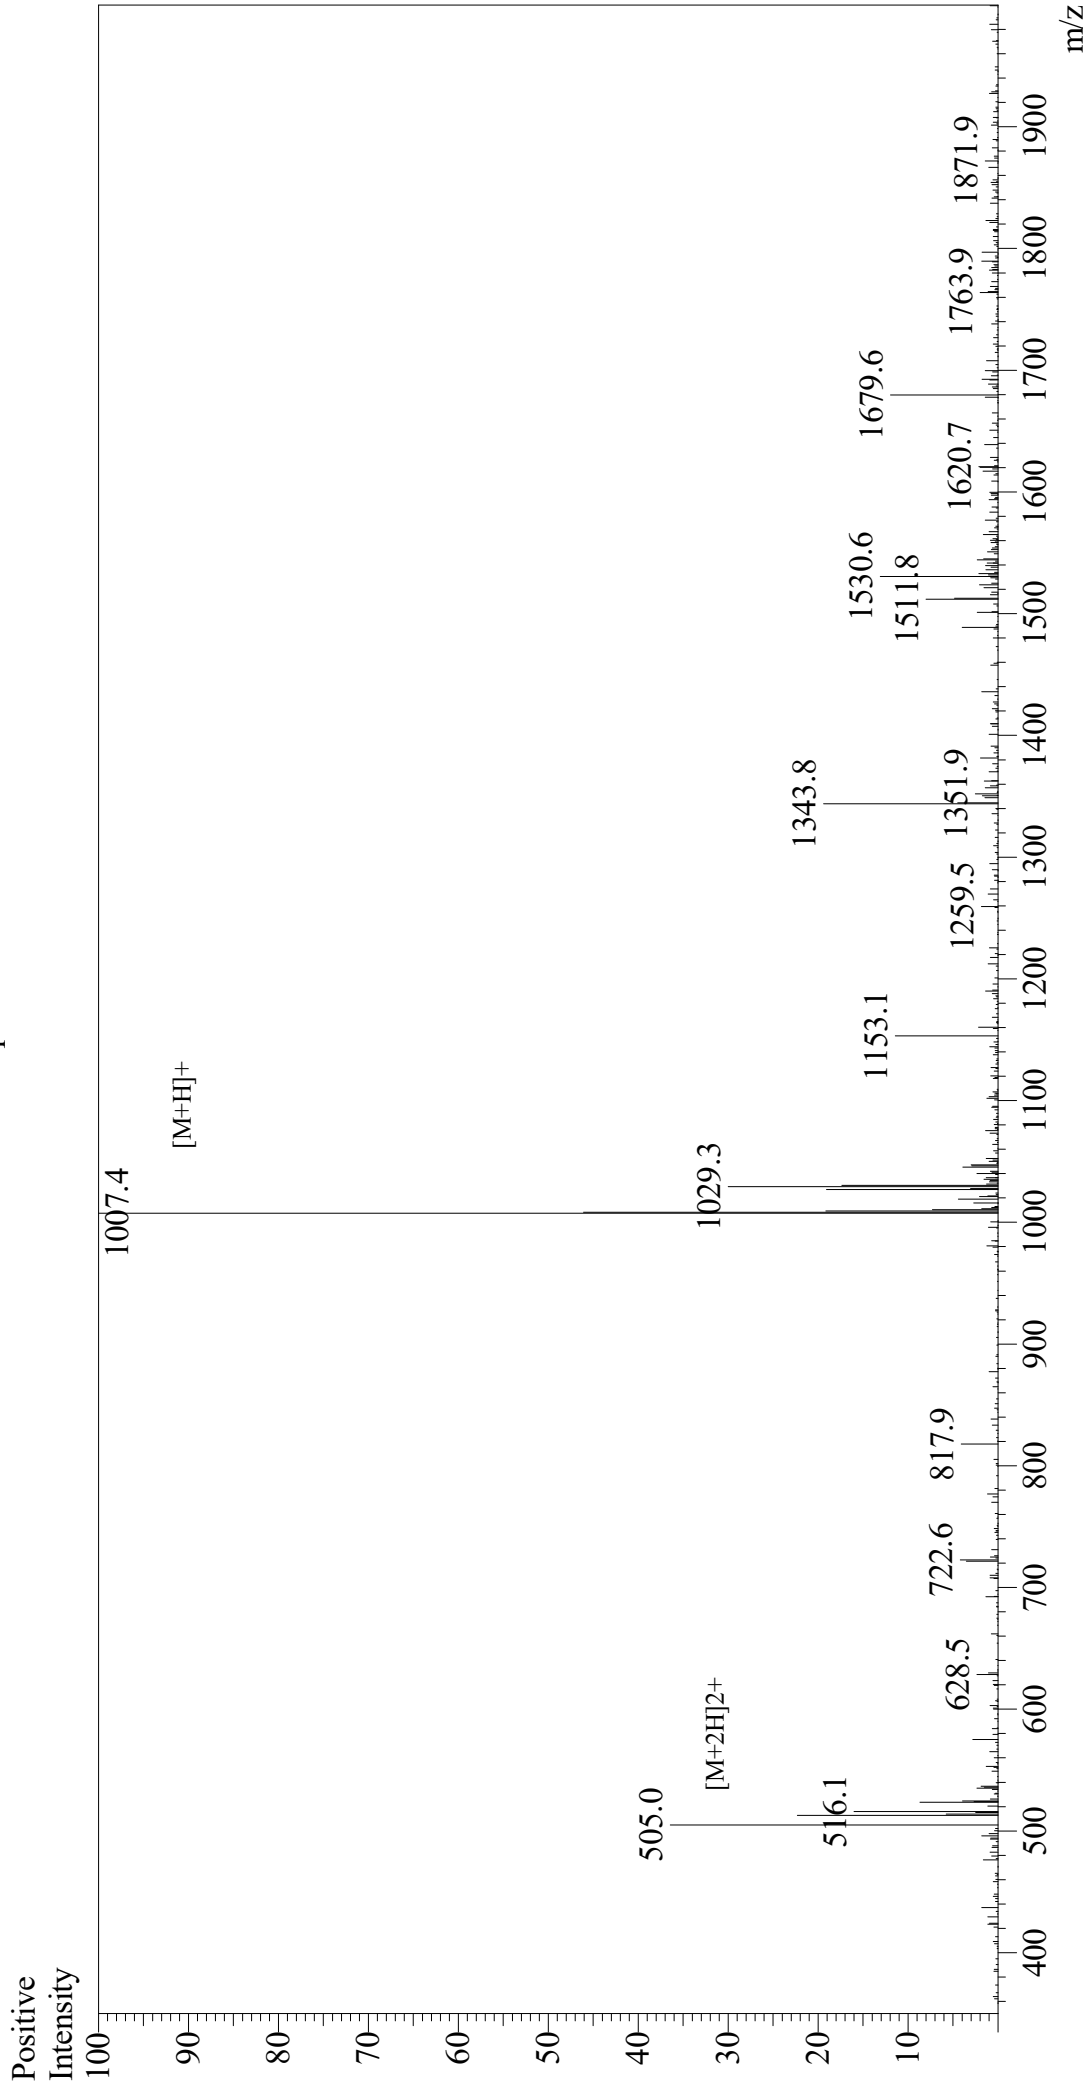

## Sample Information

Month-Day Processed : 05/07/21  
 Time Processed : 12:21:37 PM  
 Injection Volume : 0.4  
 Sample Name : Oxytocin  
 Cat. No. : RP10407  
 Lot. No. : E9385821D  
 Theoretical MW : 1007.20  
 Observed MW : 1006.4

## Interface

Interface : ESI  
 Nebulizing Gas Flow : 1.5L/min  
 CDL Temp : 250  
 Block Temp : 200

## Equipment

Equipment : GK11010007  
 Interface Bias : +4.5 kV  
 Drying Gas Flow : 5 L/min  
 T.Flow : 0.2 ml/min  
 B.conc : 50% H<sub>2</sub>O/50% MeOH