

Sample Name : IRBP(161-180)  
 Cat. No. : RP11841  
 Lot. No. : PE0821711

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow : 1 ml / min  
 Wavelength : 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

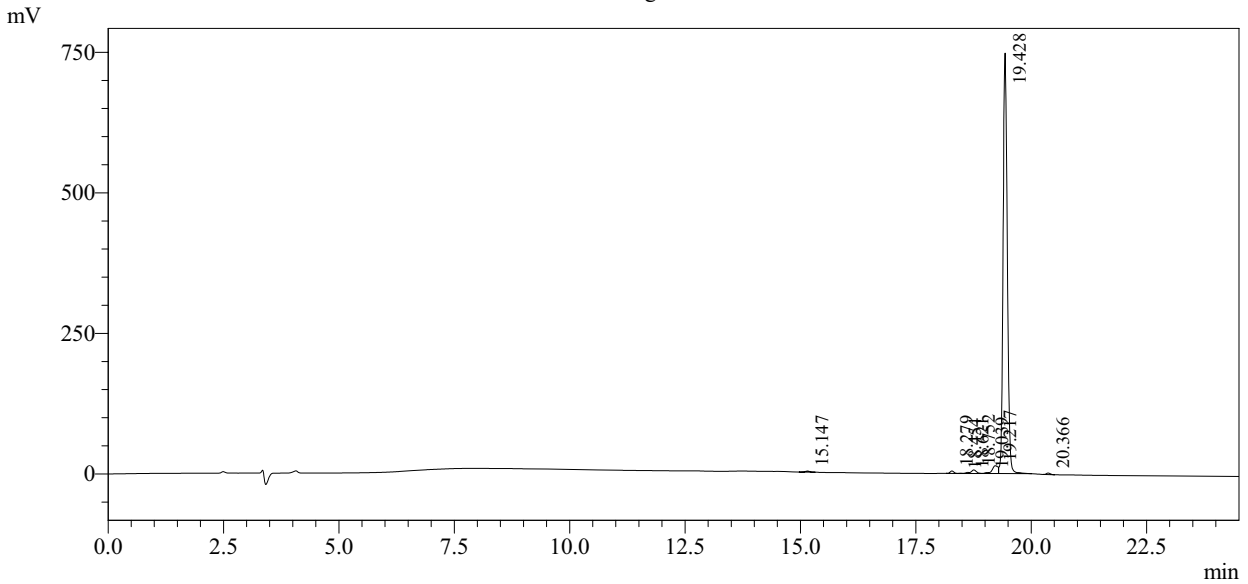

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.147	11538	2013	0.231
2	18.279	24152	4360	0.483
3	18.454	2653	410	0.053
4	18.621	9995	1911	0.200
5	18.752	46661	6432	0.933
6	19.039	9156	1691	0.183
7	19.217	115516	13938	2.310
8	19.428	4766264	747966	95.292
9	20.366	15813	2722	0.316
Total		5001747	781442	100.000