

Sample Name :C-Peptide (3-33), human
 Cat No.: RP11116
 Lot No.:E7267520B
 Time Processed :8:50:25
 Month-Day-Year Processed :02/06/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

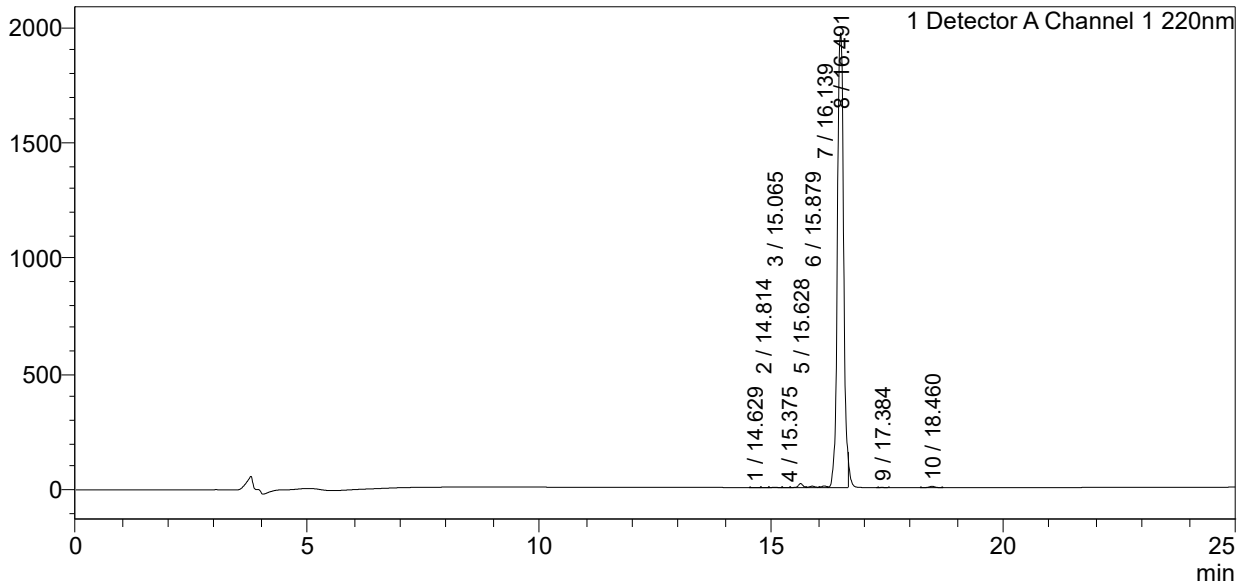

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.629	700	107	0.004
2	14.814	371	74	0.002
3	15.065	10135	1352	0.055
4	15.375	2448	257	0.013
5	15.628	122120	17571	0.657
6	15.879	52781	6459	0.284
7	16.139	56178	7293	0.302
8	16.491	18292556	1966540	98.429
9	17.384	3332	554	0.018
10	18.460	43830	5456	0.236
Total		18584451	2005664	100.000