

Sample Name :OVA G4 peptide
 Cat No. :RP20398
 Lot No. :E4840921G
 Time Processed :0:48:19
 Month-Day-Year Processed :07/22/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

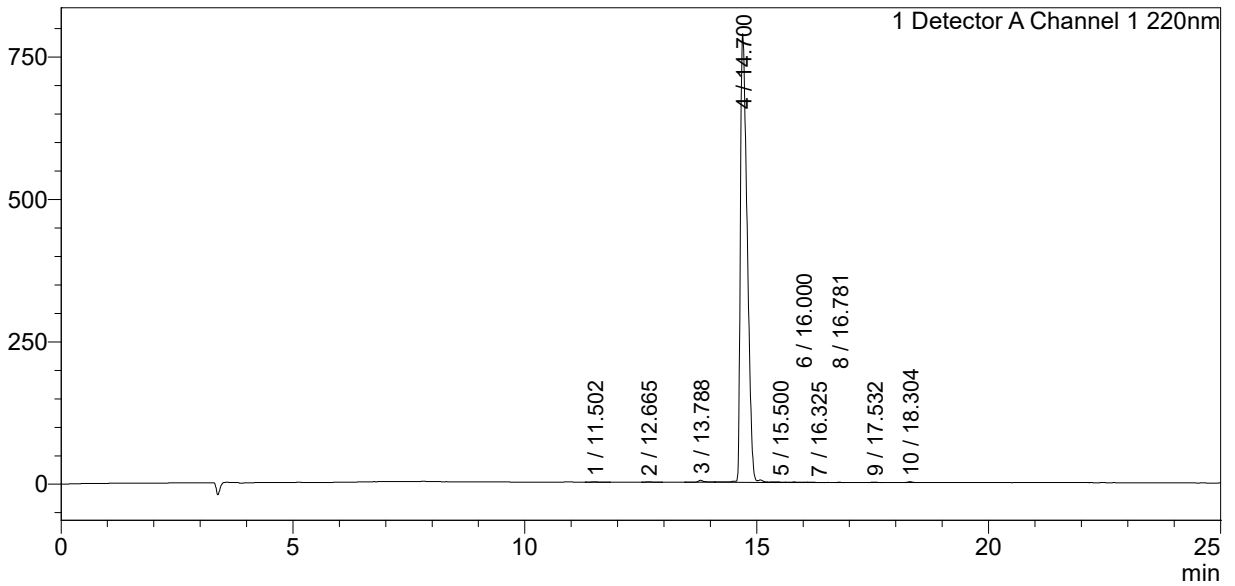

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.502	6166	632	0.076
2	12.665	5021	553	0.062
3	13.788	38405	3627	0.472
4	14.700	8039410	779636	98.775
5	15.500	14413	706	0.177
6	16.000	15520	604	0.191
7	16.325	4199	196	0.052
8	16.781	2443	429	0.030
9	17.532	4574	575	0.056
10	18.304	8948	1304	0.110
Total		8139099	788260	100.000