

Sample Name: Bacterial Sortase Substrate III, Abz/DNP
 Cat No.: RP20431
 Lot No.: E6205820A
 Time Processed : 9:44:46
 Month-Day-Year Processed : 01/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
45.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

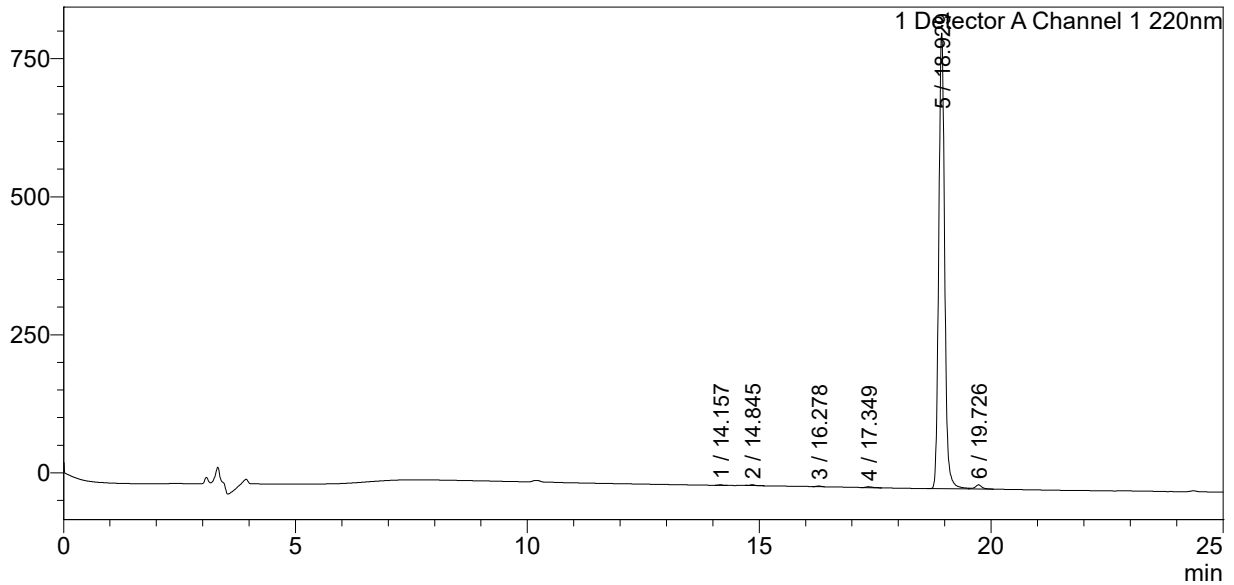

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.157	6334	1080	0.085
2	14.845	11752	1803	0.159
3	16.278	9062	1425	0.122
4	17.349	14222	1536	0.192
5	18.929	7293440	825493	98.438
6	19.726	74355	7407	1.004
Total		7409165	838744	100.000