


Mass Spectrum

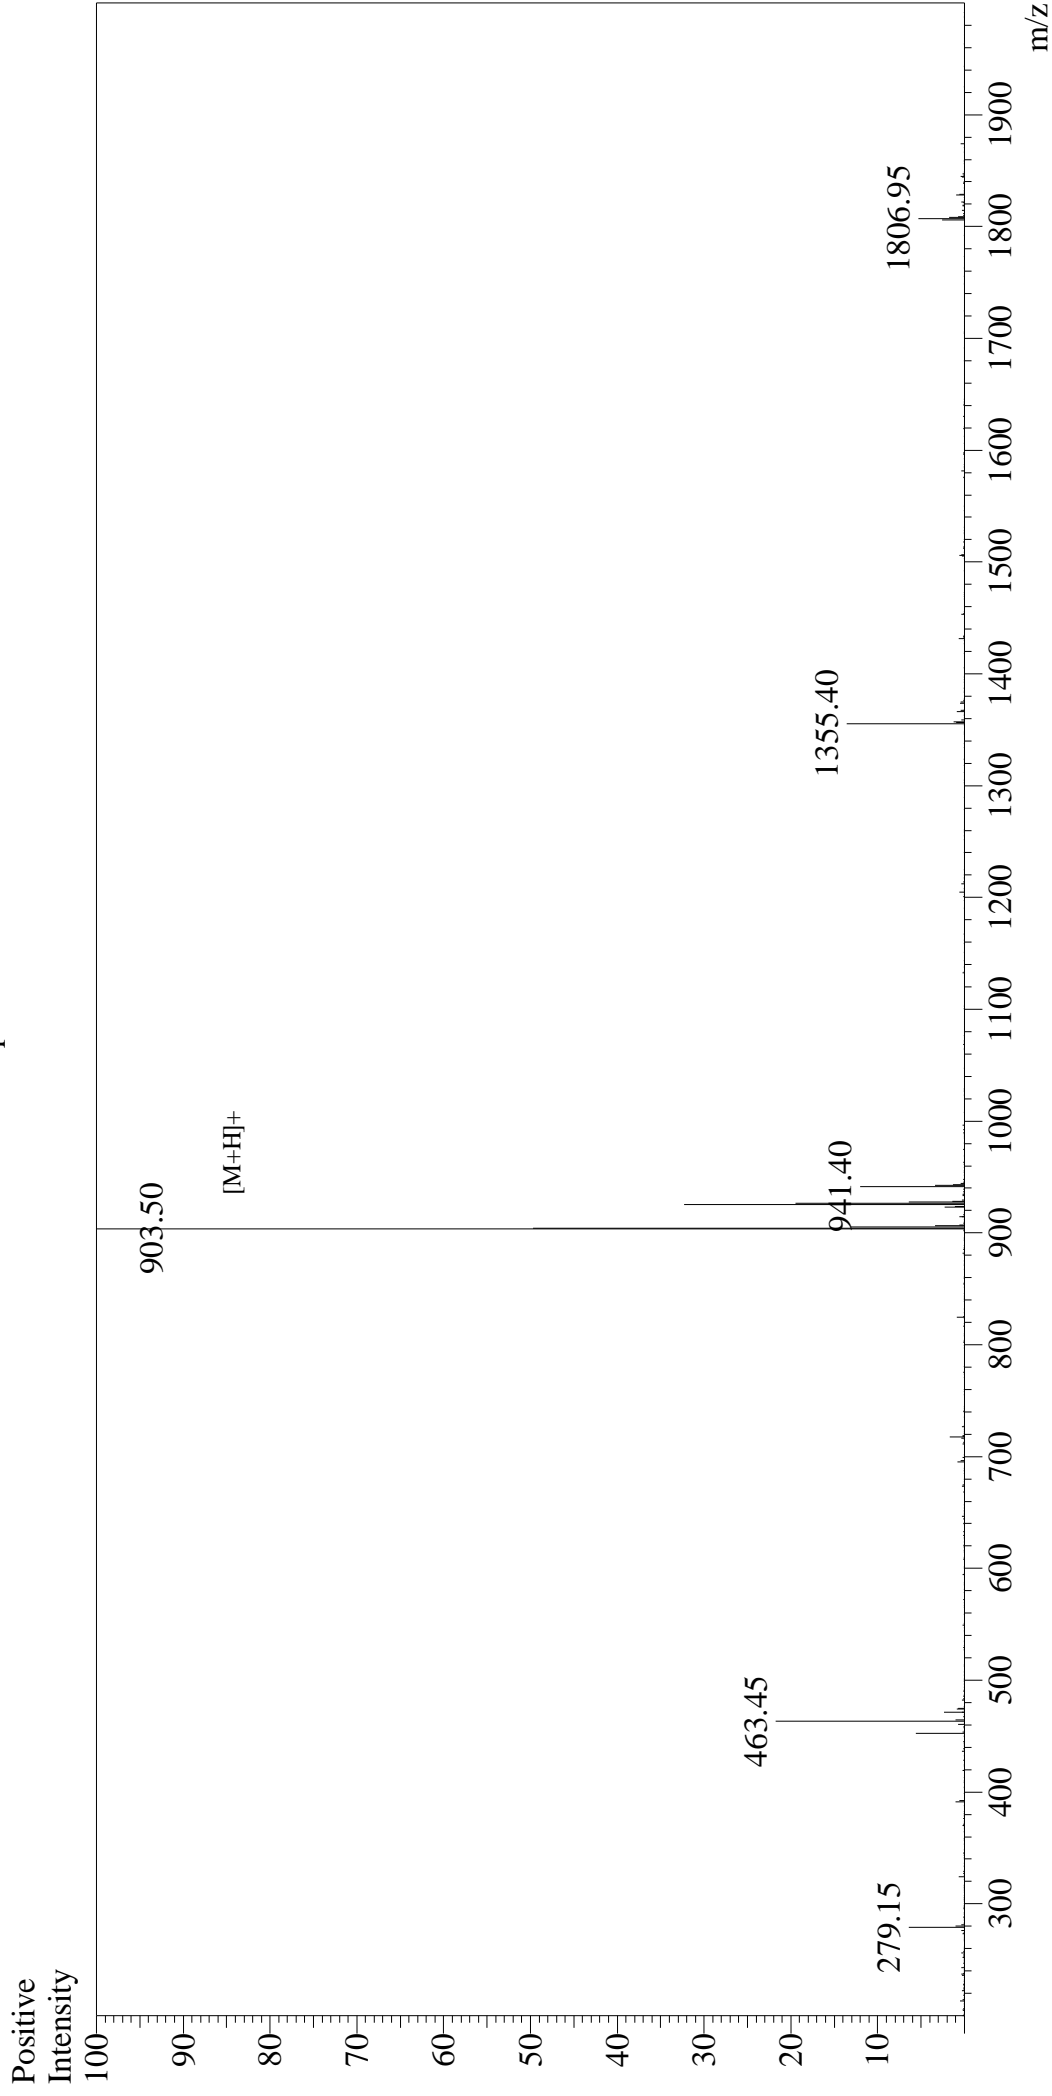

Sample Information

User : Gary
Month-Day Processed : 12/31/16
Time Processed : 10:35:24
Injection Volume : 1
Sample Name : Rhodopsin Epitope Tag
Cat No. : RP20400
Lot No. : 8173334570002/PE0594
Theoretical MW : 902.95
Observed MW : 902.50

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH