

Sample Name : PACAP (1-27), human, ovine, rat  
 Cat No. : RP10334  
 Lot No. : E4709019I  
 Time Processed : 10:01:13 AM  
 Month-Day-Year Processed : 09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

### <Chromatogram>

mV

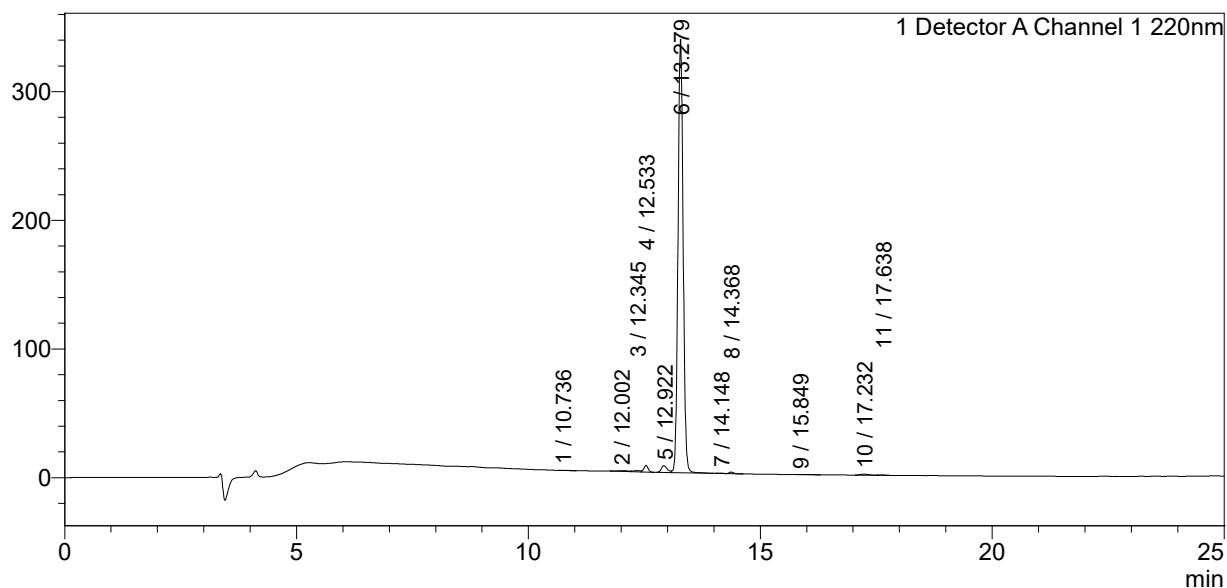

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.736	1105	94	0.040
2	12.002	10997	556	0.403
3	12.345	10432	1001	0.382
4	12.533	32915	5224	1.206
5	12.922	46726	5282	1.712
6	13.279	2603296	337148	95.387
7	14.148	1692	263	0.062
8	14.368	8068	1242	0.296
9	15.849	2190	110	0.080
10	17.232	9781	782	0.358
11	17.638	1986	264	0.073
Total		2729189	351965	100.000