


Mass Spectrum

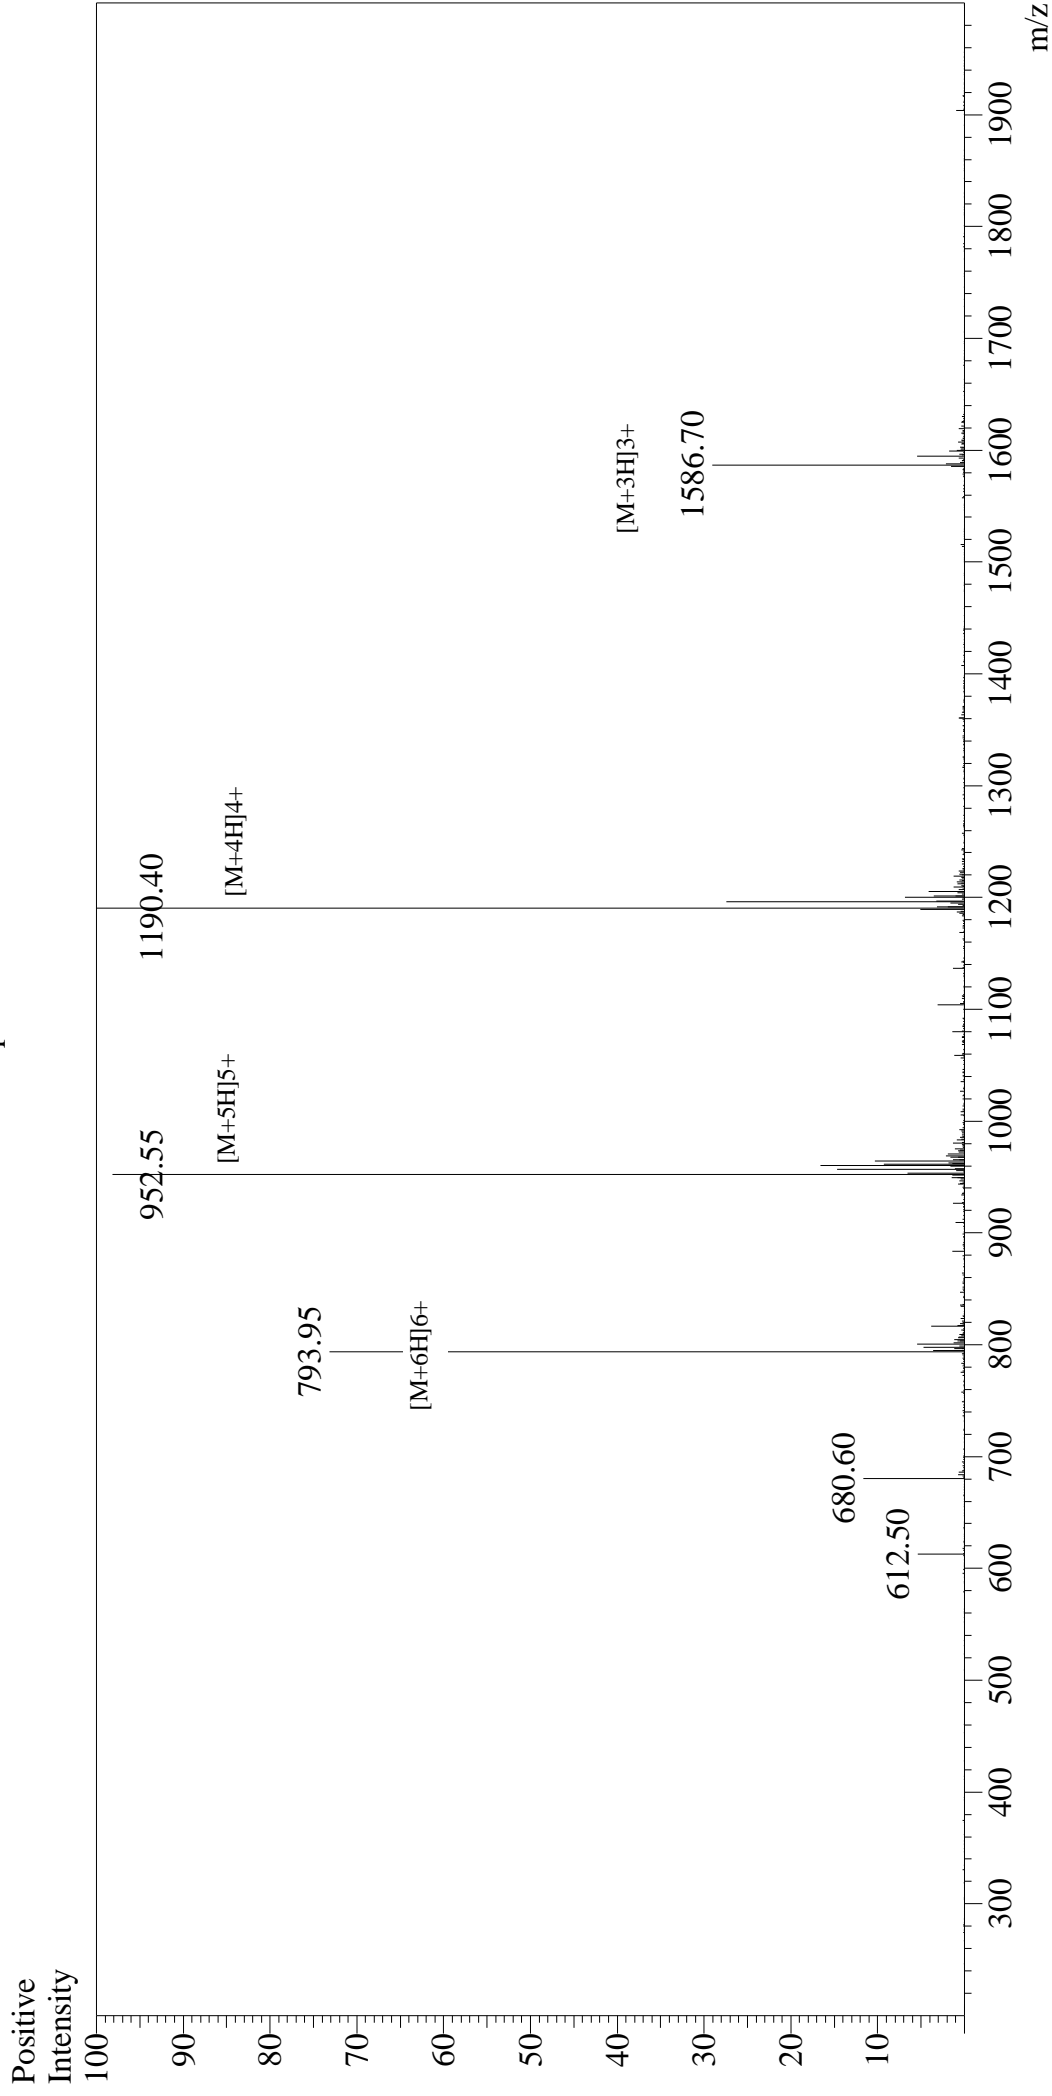

Sample Information

User : Gary
Month-Day Processed : 12/14/16
Time Processed : 9:44:33
Injection Volume : 1
Sample Name : Corticotropin Releasing Factor, human, rat
Cat No. : RPI0982
Lot No. : PE3451612
Theoretical MW : 4757.45
Observed MW : 4757.60

Interface

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH