

Sample Name : Cortistatin 14, human, rat
 Cat. No. : RP10972
 Lot. No. : PE7251702

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
32.00	Pumps	Pump A B.Conc	95	
32.01	Pumps	Pump A B.Conc	5	
50.00	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

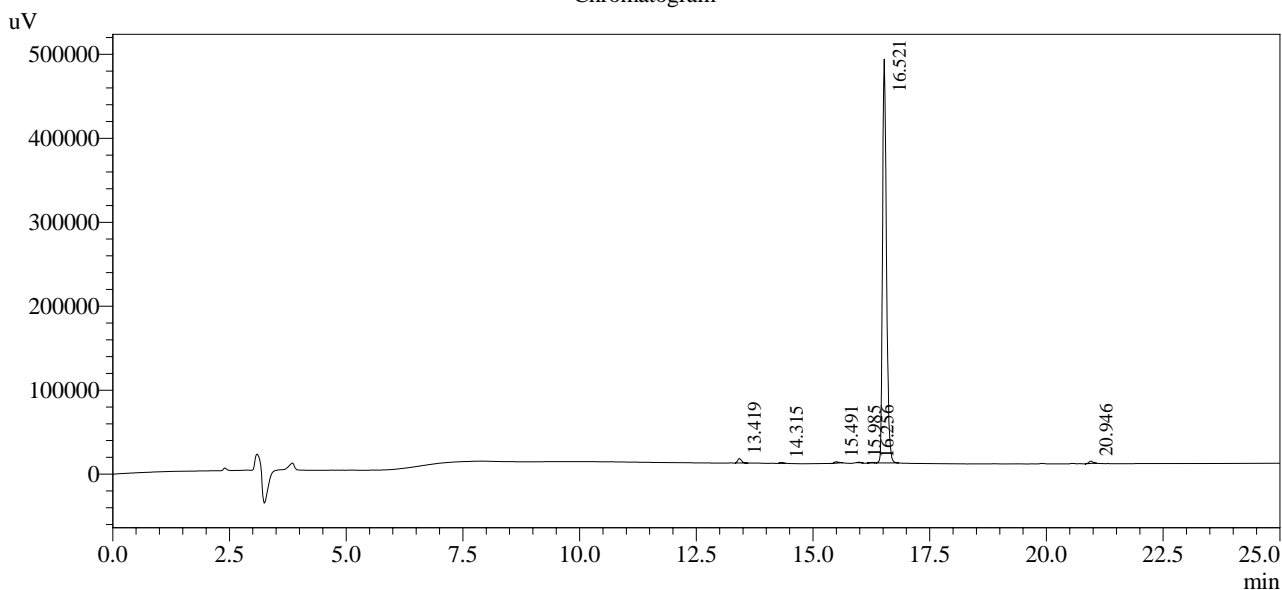

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.419	29865	5342	1.027
2	14.315	3210	744	0.110
3	15.491	10048	1594	0.345
4	15.985	3076	743	0.106
5	16.256	3892	702	0.134
6	16.521	2842485	481020	97.721
7	20.946	16210	2763	0.557
Total		2908785	492908	100.000