

Sample Name :Bacterial Sortase Substrate III, Abz/DNP
 Cat No.:RP20431
 Lot No.:E0330020B
 Time Processed :15:16:57
 Month-Day-Year Processed :02/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
30.00	Pumps	Pump A B.Conc	95
35.00	Pumps	Pump A B.Conc	95
35.10	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
45.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

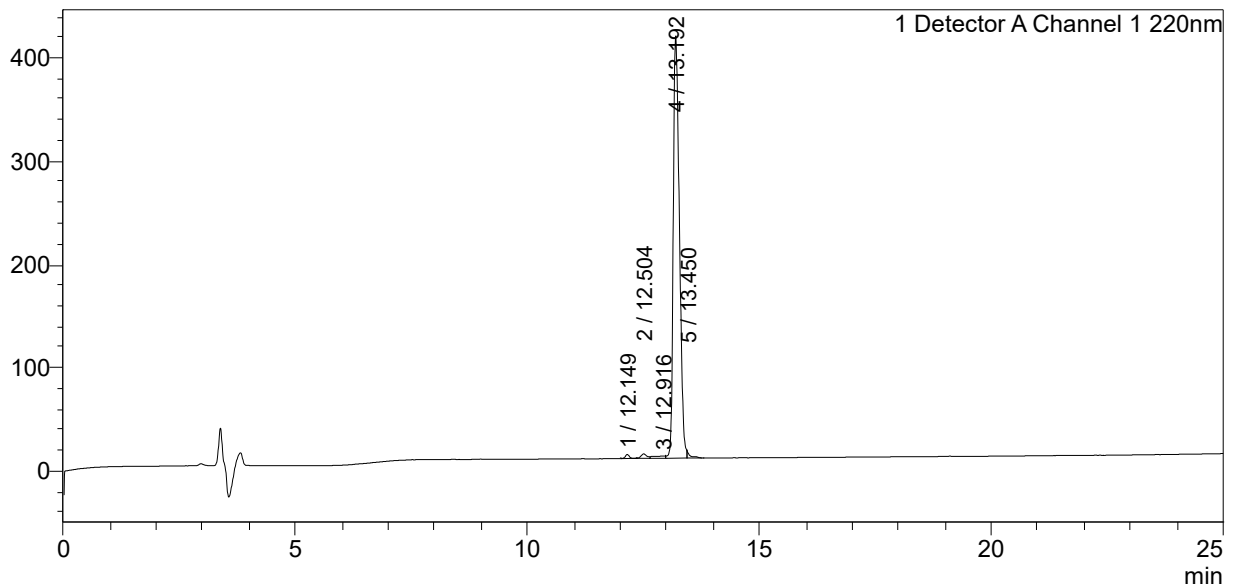

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.149	23753	3916	0.612
2	12.504	36989	4444	0.953
3	12.916	44374	2186	1.143
4	13.192	3746717	408643	96.524
5	13.450	29803	6113	0.768
Total		3881636	425302	100.000