

Sample Name :Influenza HA (518-526)  
 Cat. No. :RP20284  
 Lot. No. :PE1791811  
 Time Processed : 10:06:17  
 Month-Day-Year Processed : 11/19/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

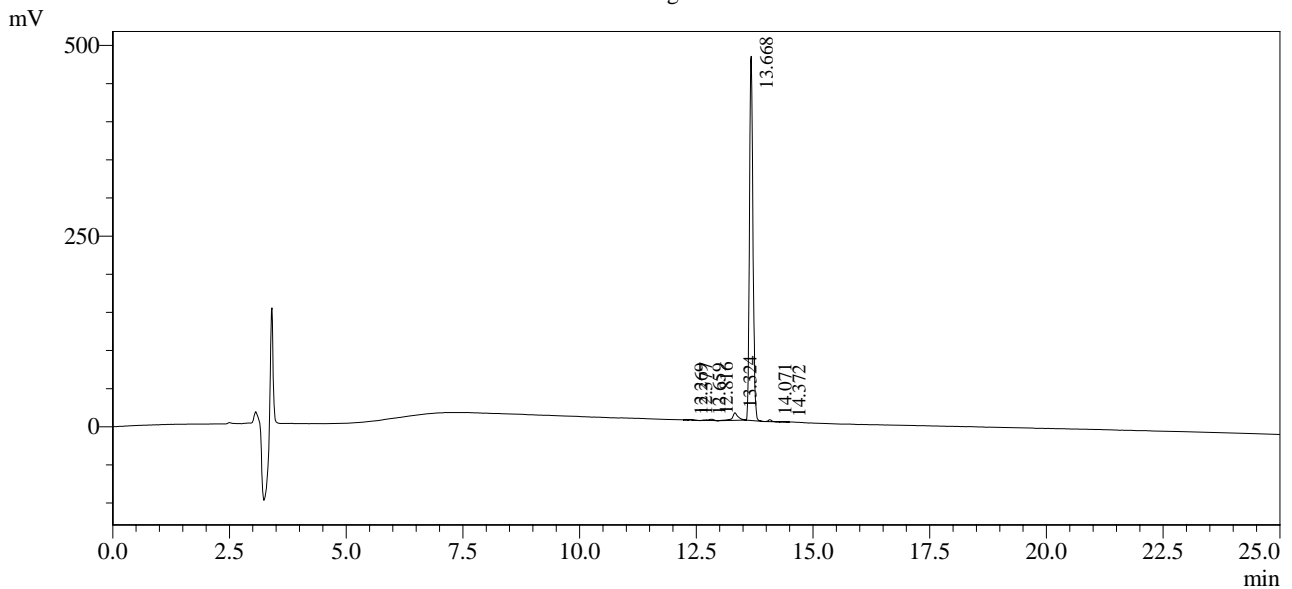

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.269	250	92	0.010
2	12.377	4051	692	0.156
3	12.659	949	268	0.037
4	12.816	11023	1582	0.425
5	13.324	87772	10032	3.384
6	13.668	2474485	477699	95.412
7	14.071	13543	2616	0.522
8	14.372	1389	221	0.054
Total		2593461	493202	100.000