

Sample Name :Influenza Hemagglutinin(307-319)
 Cat No. :RP20087
 Lot No. :PE0931812
 Time Processed :14:55:05
 Month-Day-Year Processed :12/22/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

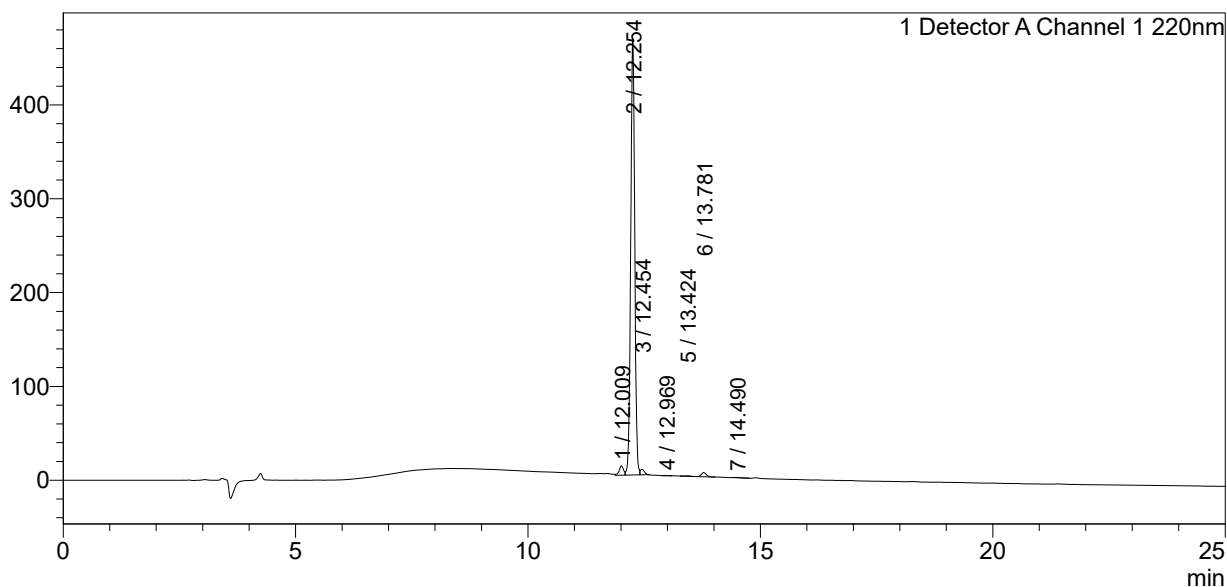

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.009	66817	10065	2.276
2	12.254	2793178	465208	95.130
3	12.454	34217	5891	1.165
4	12.969	1722	300	0.059
5	13.424	5249	660	0.179
6	13.781	32336	4400	1.101
7	14.490	2635	380	0.090
Total		2936154	486904	100.000