

Sample Name : γ -1-Melanocyte Stimulating Hormone (MSH), amide
 Cat. No. : RP10650
 Lot. No. : E4762619I
 Time Processed :14:12:36
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010009

Chromatogram

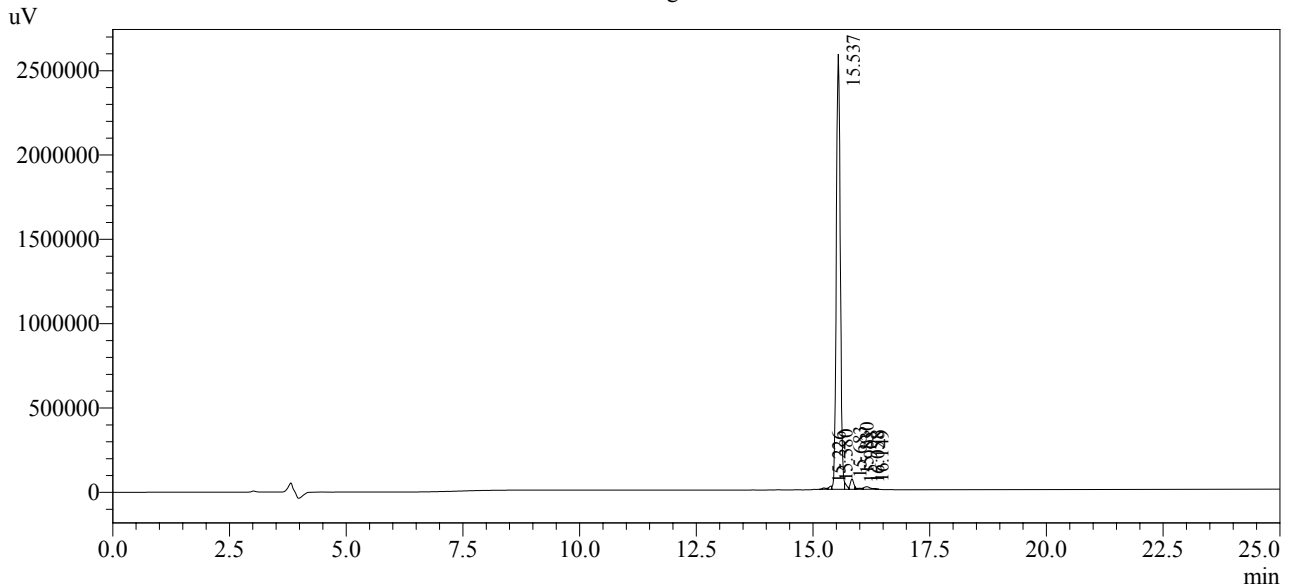

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.226	54904	8201	0.344
2	15.380	75245	18771	0.471
3	15.537	15223803	2579240	95.281
4	15.683	116394	37842	0.728
5	15.830	304926	60347	1.908
6	15.908	15740	10924	0.099
7	16.058	45017	6131	0.282
8	16.149	141841	14696	0.888
Total		15977870	2736153	100.000