


# Mass Spectrum

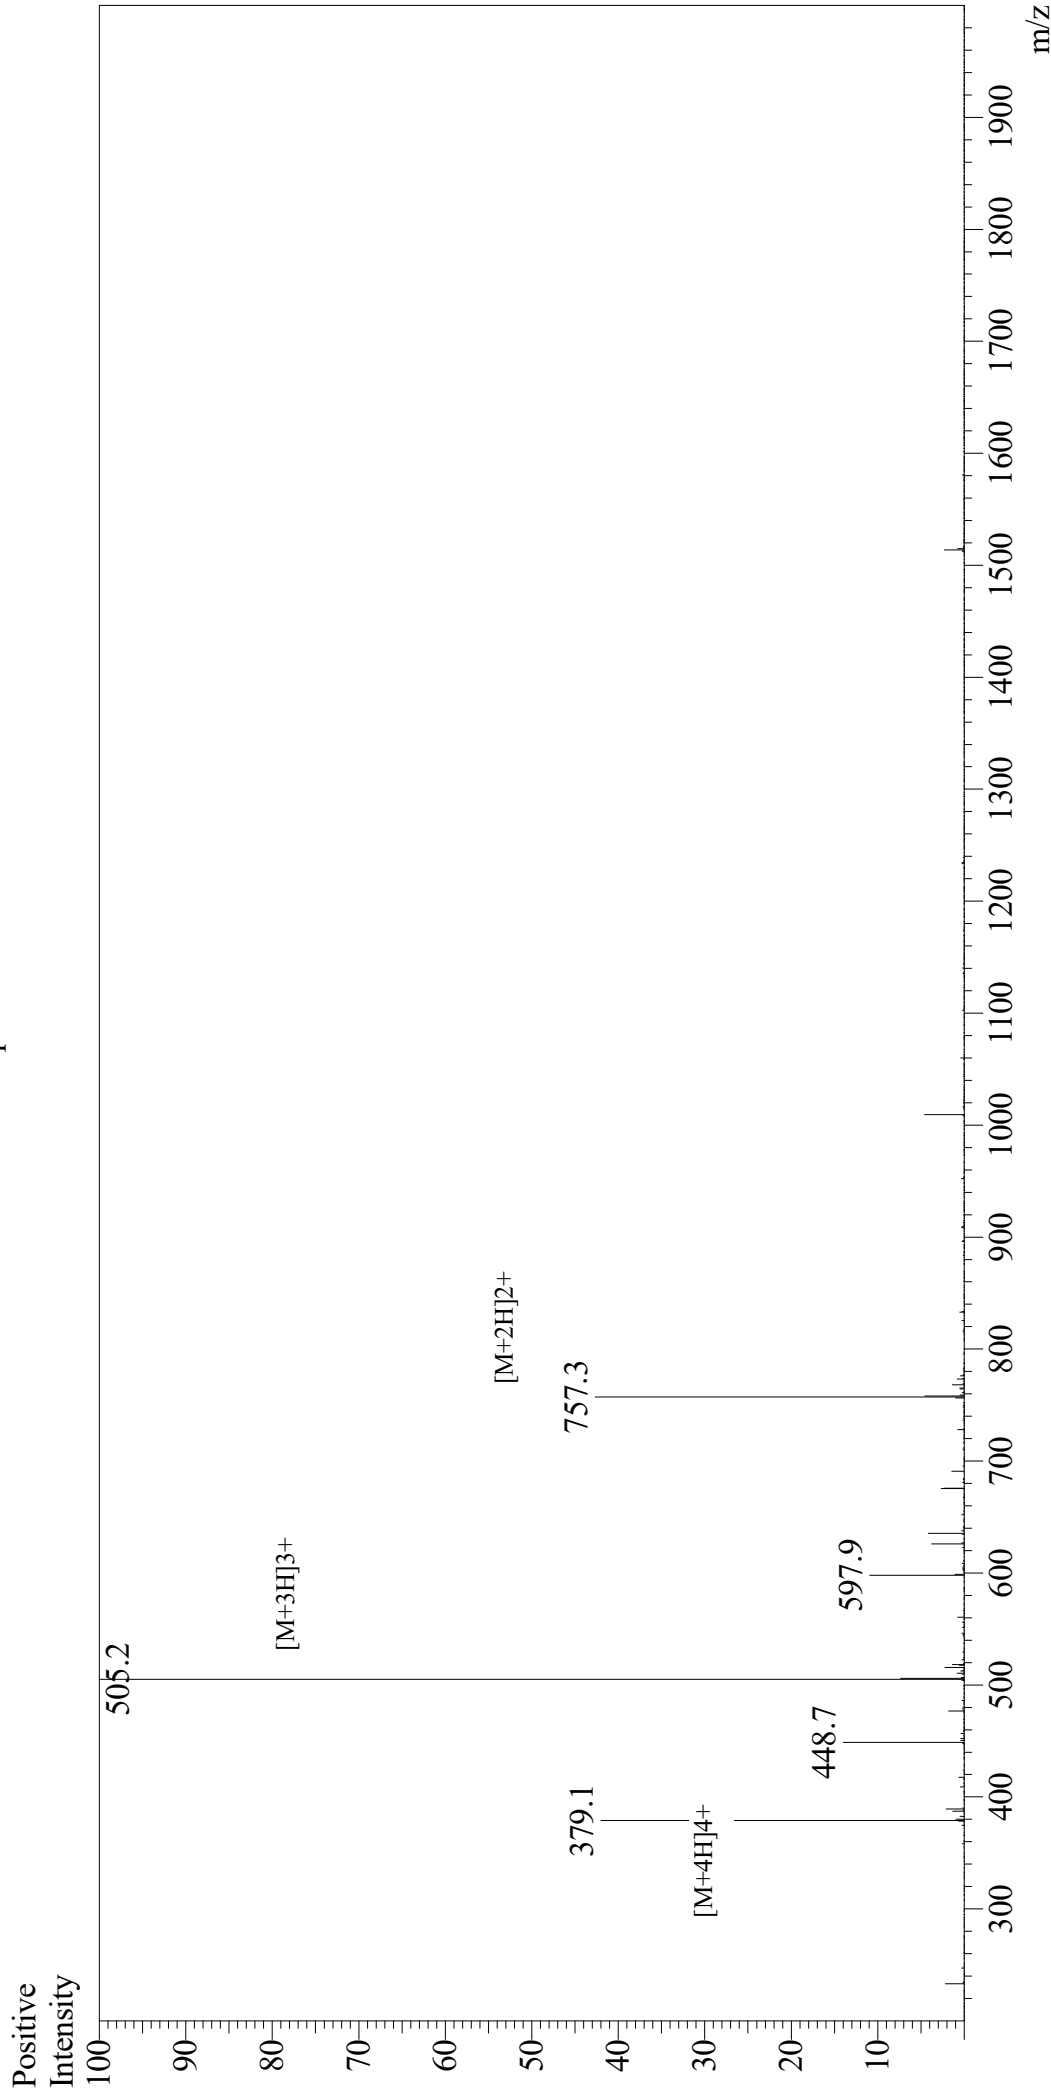

Sample Information  
User : Gary  
Month-Day Processed : 09/18/19  
Time Processed : 08:21:44 PM  
Injection Volume : 0.3  
Sample Name :  $\gamma$ -1-Melanocyte Stimulating Hormone (MSH), amide  
Cat No. : RP10650  
Lot No. : E4762619I  
Theoretical MW : 1512.90  
Observed MW : 1512.6

Equipment : GK11010007  
Interface Bias : +4.5kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200