

Sample Name : Bombesin
 Cat. No. : RP 11157
 Lot. No. : PE5521610

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

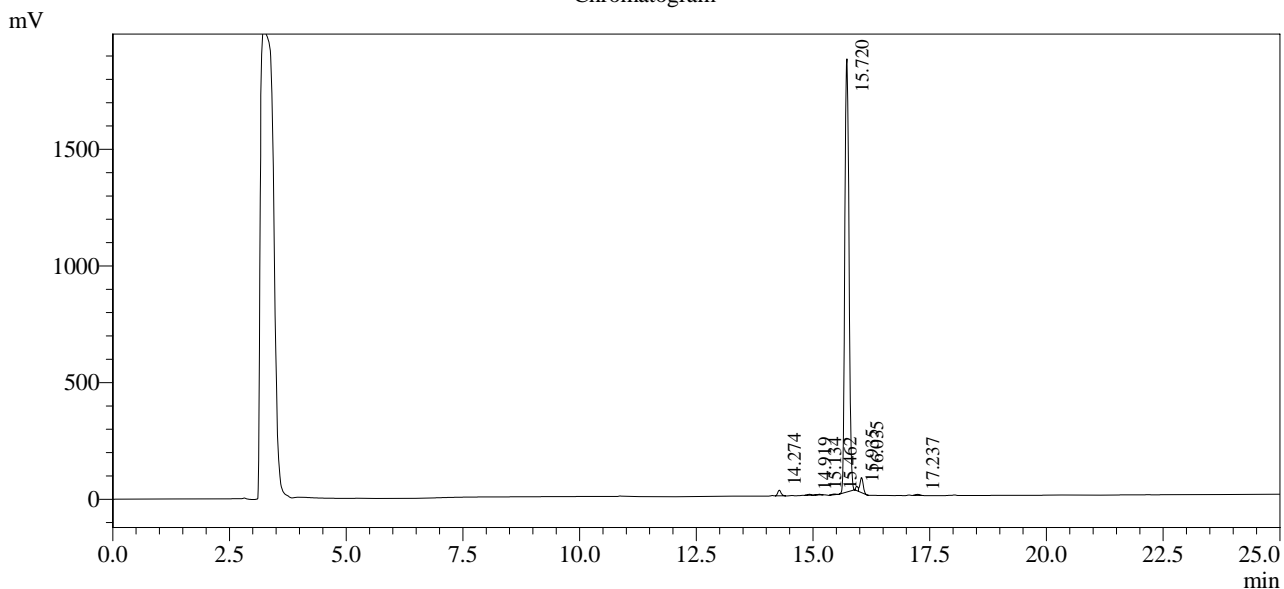

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.274	119321	24083	0.982
2	14.919	20411	4018	0.168
3	15.134	13014	2816	0.107
4	15.462	19002	2795	0.156
5	15.720	11581433	1856743	95.313
6	15.935	65738	18189	0.541
7	16.035	301523	64390	2.481
8	17.237	30565	4647	0.252
Total		12151006	1977680	100.000