

Sample Name :HA Peptide  
 Cat No :RP11735  
 Lot No :E7887220L  
 Time Processed :1:17:25 PM  
 Month-Day-Year Processed :12/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: GK11010011

<Chromatogram>

mV

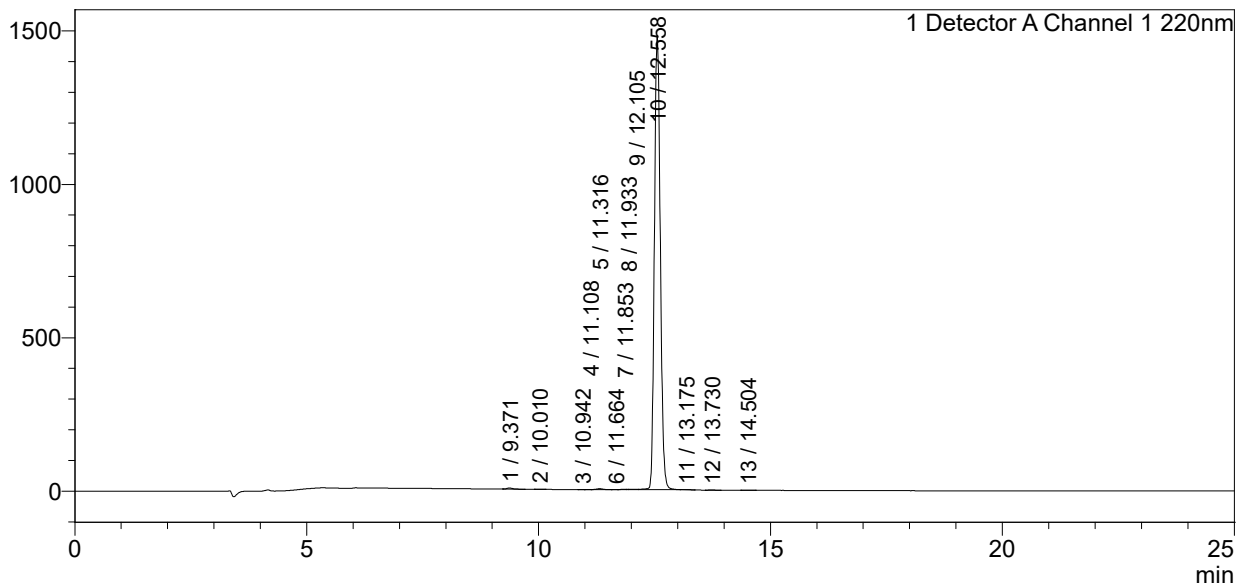

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.371	32709	3885	0.246
2	10.010	1744	239	0.013
3	10.942	1550	277	0.012
4	11.108	2889	363	0.022
5	11.316	28967	2963	0.218
6	11.664	3032	612	0.023
7	11.853	9133	1035	0.069
8	11.933	3203	1114	0.024
9	12.105	18696	1749	0.141
10	12.558	13164994	1480591	99.151
11	13.175	3343	356	0.025
12	13.730	5519	624	0.042
13	14.504	1886	313	0.014
Total		13277665	1494120	100.000