

Sample Name :Xenopsin
Cat No. :RP10479
Lot No. :E4799719I
Time Processed :15:03:26
Month-Day-Year Processed :09/26/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ17010508

<Chromatogram>

mV

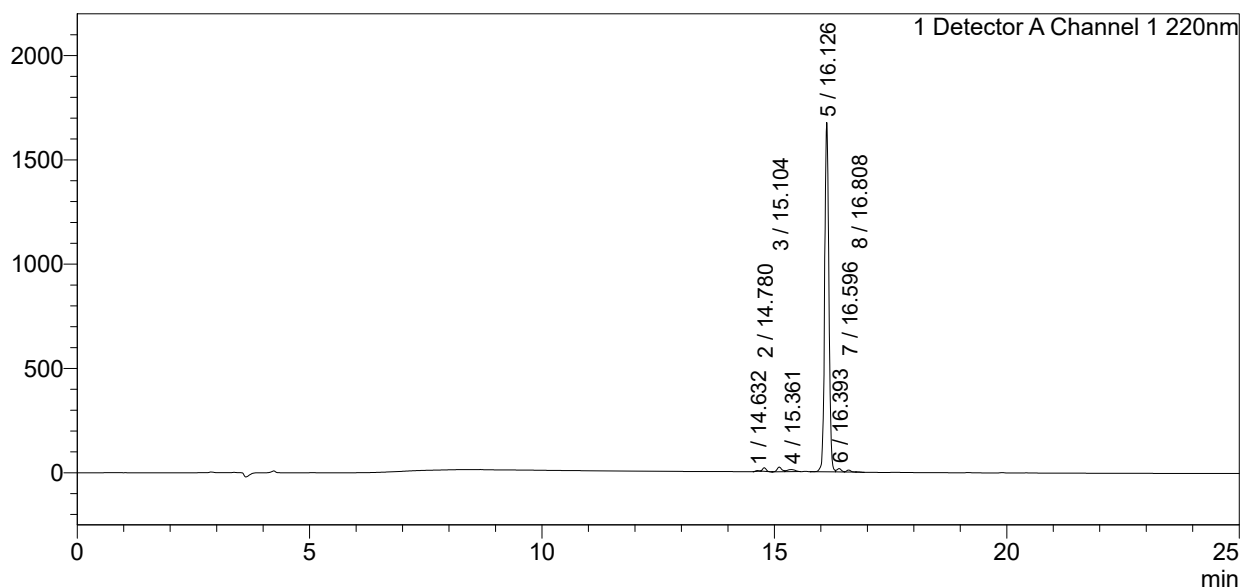

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.632	16873	3689	0.153
2	14.780	83555	16703	0.757
3	15.104	156194	22731	1.414
4	15.361	117262	9847	1.062
5	16.126	10506021	1674987	95.139
6	16.393	102903	16200	0.932
7	16.596	56708	9510	0.514
8	16.808	3273	672	0.030
Total		11042789	1754339	100.000