

Sample Name :Autocamtide 2-amide  
 Cat No. :RP20277  
 Lot No. :E5457719G  
 Time Processed :6:13:08  
 Month-Day-Year Processed :07/07/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ17010508

<Chromatogram>

mV

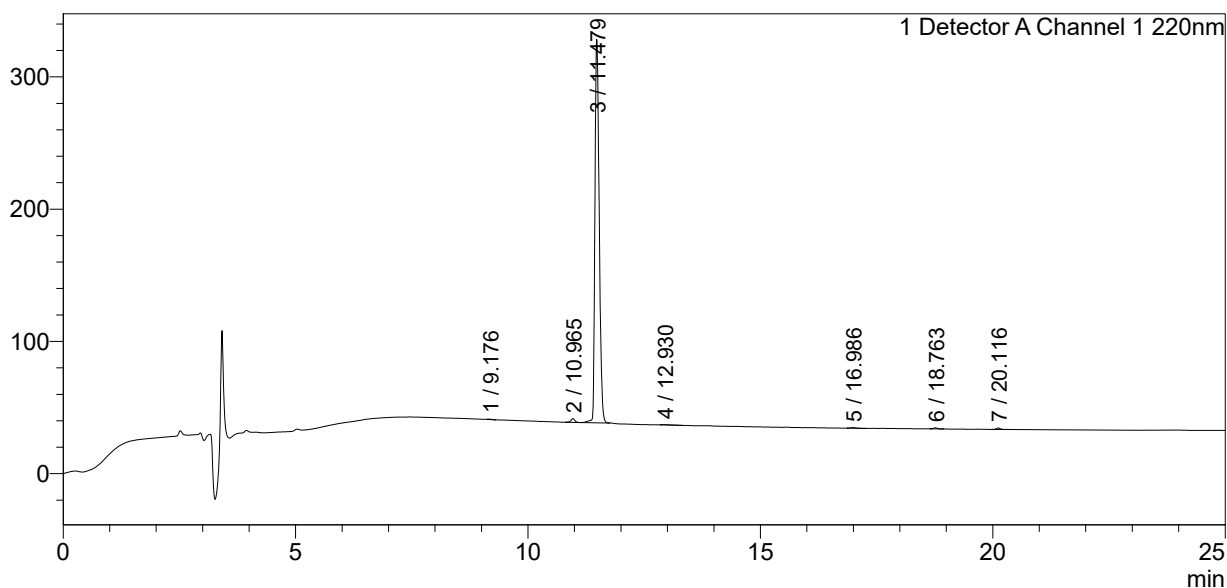

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.176	1525	346	0.081
2	10.965	15938	2864	0.846
3	11.479	1849543	289911	98.163
4	12.930	2676	289	0.142
5	16.986	3200	470	0.170
6	18.763	4804	806	0.255
7	20.116	6471	1111	0.343
Total		1884157	295796	100.000