


# Mass Spectrum

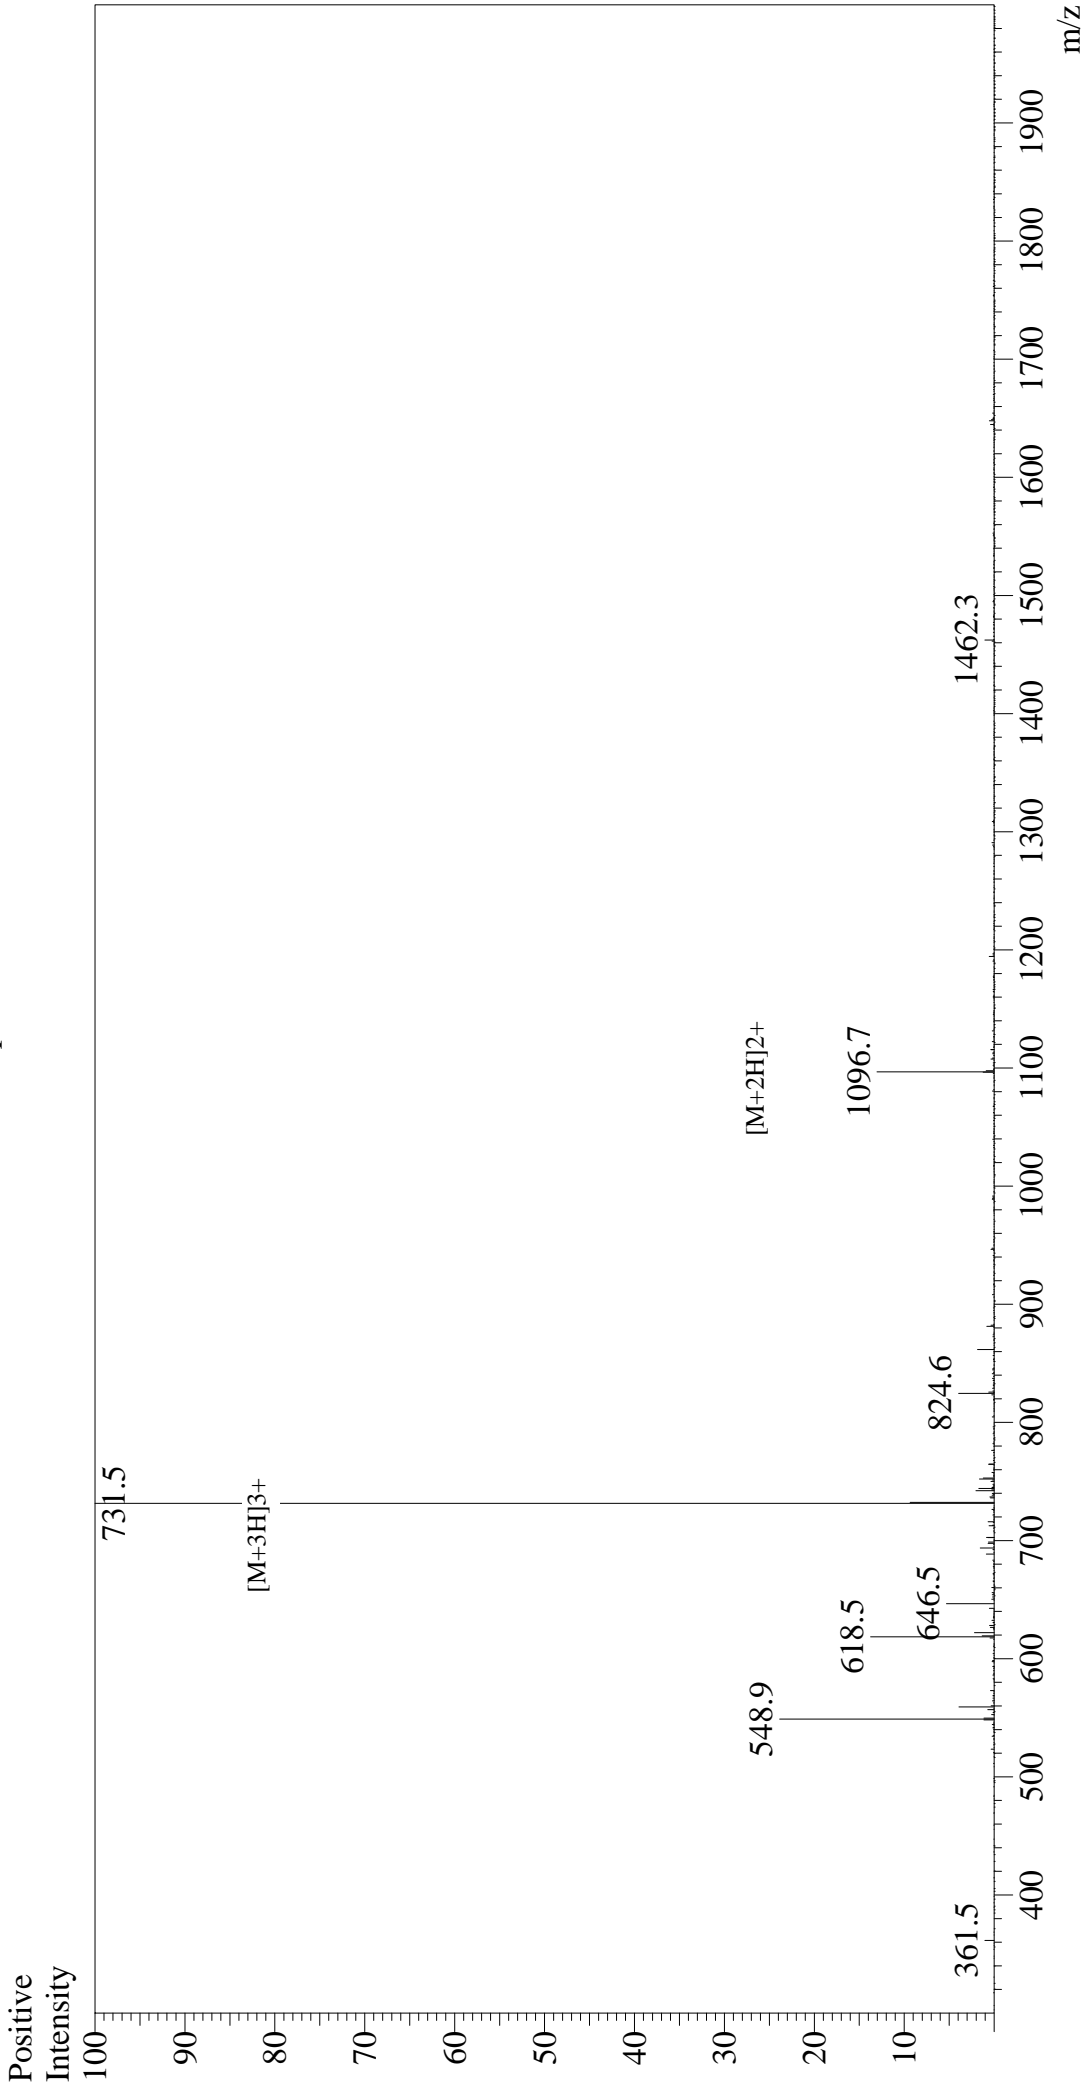

## Sample Information

Acquired by :	Gary	Equipment	: GK11010007
Month-Day Processed :	08/13/19	Interface Bias	: +4.5 kV
Time Processed :	22:32:12	Drying Gas Flow	: 5 L/min
Injection Volume :	0.3	T.Flow	: 0.2 ml/min
Sample Name :	Mycobacterium tuberculosis Protein Ag85A	B.conc	: 50% H <sub>2</sub> O/50% MeOH
Cat. No. :	RP20202		
Lot. No. :	E6646119H		
Theoretical MW :	2191.50		
Observed MW :	2191.5		

Interface	: ESI
Nebulizing Gas Flow	: 1.5L/min
CDL Temp	: 250
Block Temp	: 200