

Sample Name : CEF1, Influenza Matrix Protein M1 (58 - 66)
 Cat.No : RP19978
 Lot.No : E7696720G
 Time Processed: 4:30:20
 Year-Month-Day: 2020/7/25

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010015

<Chromatogram>

mV

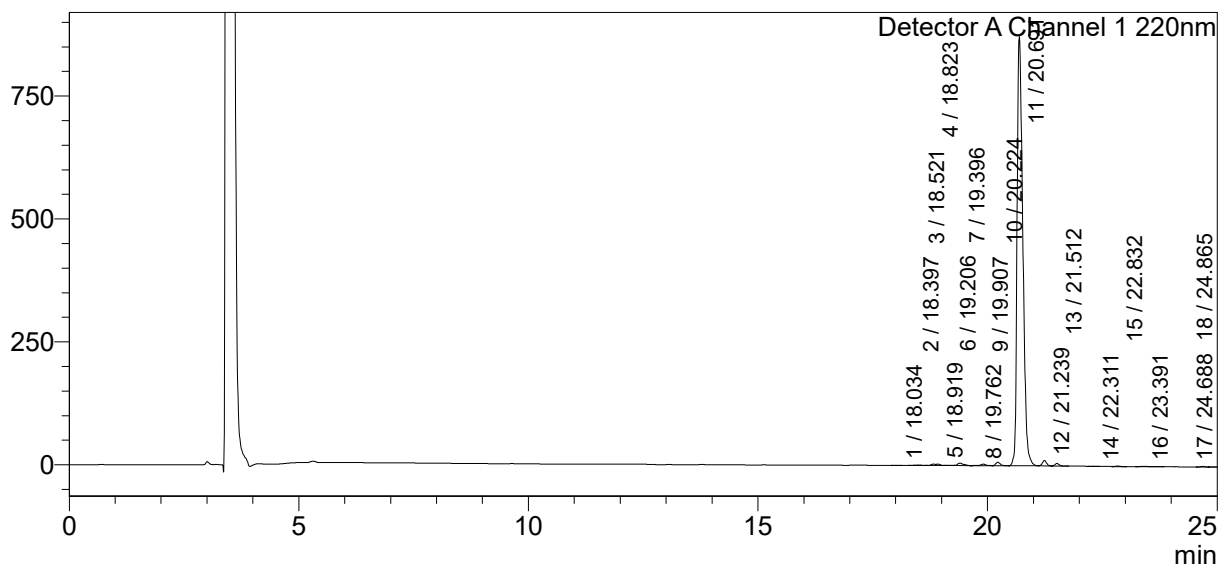

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	18.034	1522	189	0.019
2	18.397	3199	539	0.040
3	18.521	6287	899	0.080
4	18.823	18066	2858	0.229
5	18.919	16700	2862	0.211
6	19.206	1136	178	0.014
7	19.396	44036	5074	0.557
8	19.762	4266	689	0.054
9	19.907	23876	3231	0.302
10	20.224	46292	7124	0.586
11	20.691	7607075	872571	96.263
12	21.239	68779	10954	0.870
13	21.512	31916	5017	0.404
14	22.311	1037	154	0.013

Peak#	Ret. Time	Area	Height	Area%
15	22.832	7525	1052	0.095
16	23.391	11374	887	0.144
17	24.688	7882	1211	0.100
18	24.865	1433	203	0.018
Total		7902401	915691	100.000