

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat
 Cat No. : RP11095
 Lot No. : E4779221I
 Time Processed : 7:46:20
 Month-Day-Year Processed : 10/01/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

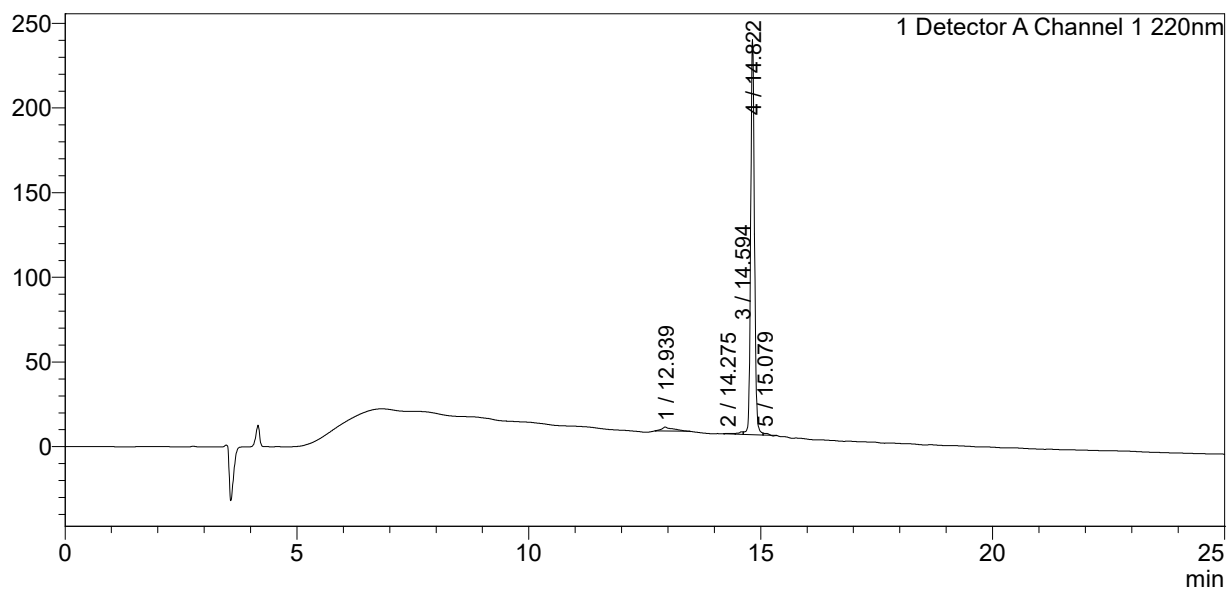

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.939	43304	2336	3.100
2	14.275	4990	346	0.357
3	14.594	10702	1540	0.766
4	14.822	1331466	227191	95.318
5	15.079	6408	1092	0.459
Total		1396870	232504	100.000