

Sample Name :mTRP-2(180-188)  
 Cat No.: RP20250  
 Lot No.: E7053919J  
 Time Processed :7:12:36  
 Month-Day-Year Processed :10/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

<Chromatogram>

mV

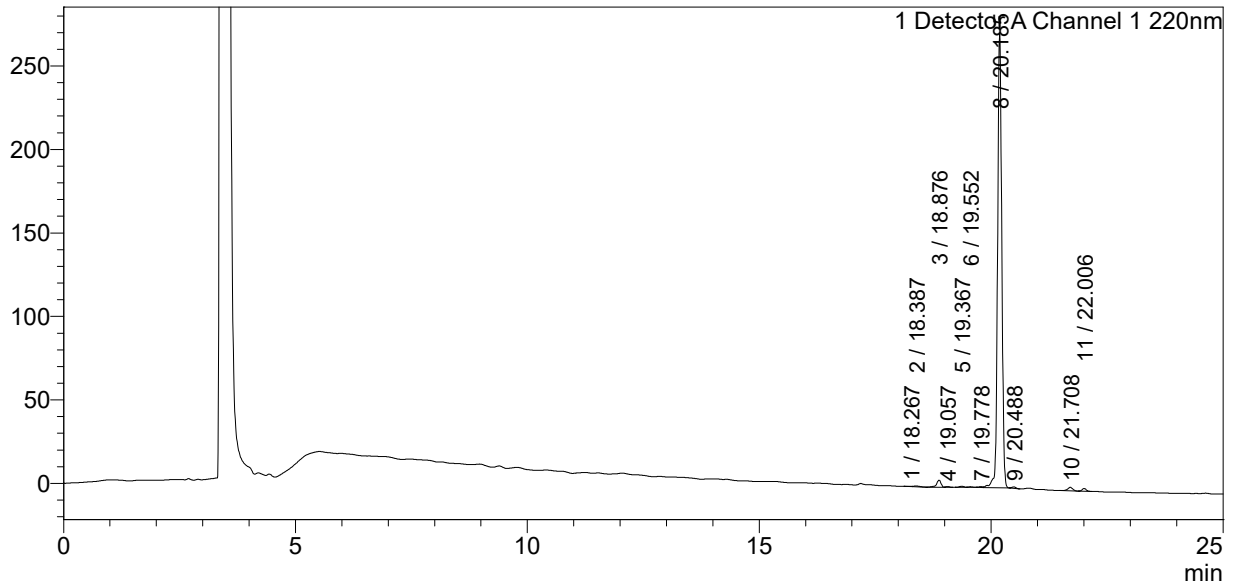

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	18.267	1702	256	0.095
2	18.387	4371	511	0.245
3	18.876	27899	4215	1.561
4	19.057	2097	449	0.117
5	19.367	4609	690	0.258
6	19.552	2479	387	0.139
7	19.778	2939	583	0.164
8	20.185	1708817	272480	95.641
9	20.488	4965	920	0.278
10	21.708	16761	2125	0.938
11	22.006	10058	1693	0.563
Total		1786697	284310	100.000