


Mass Spectrum

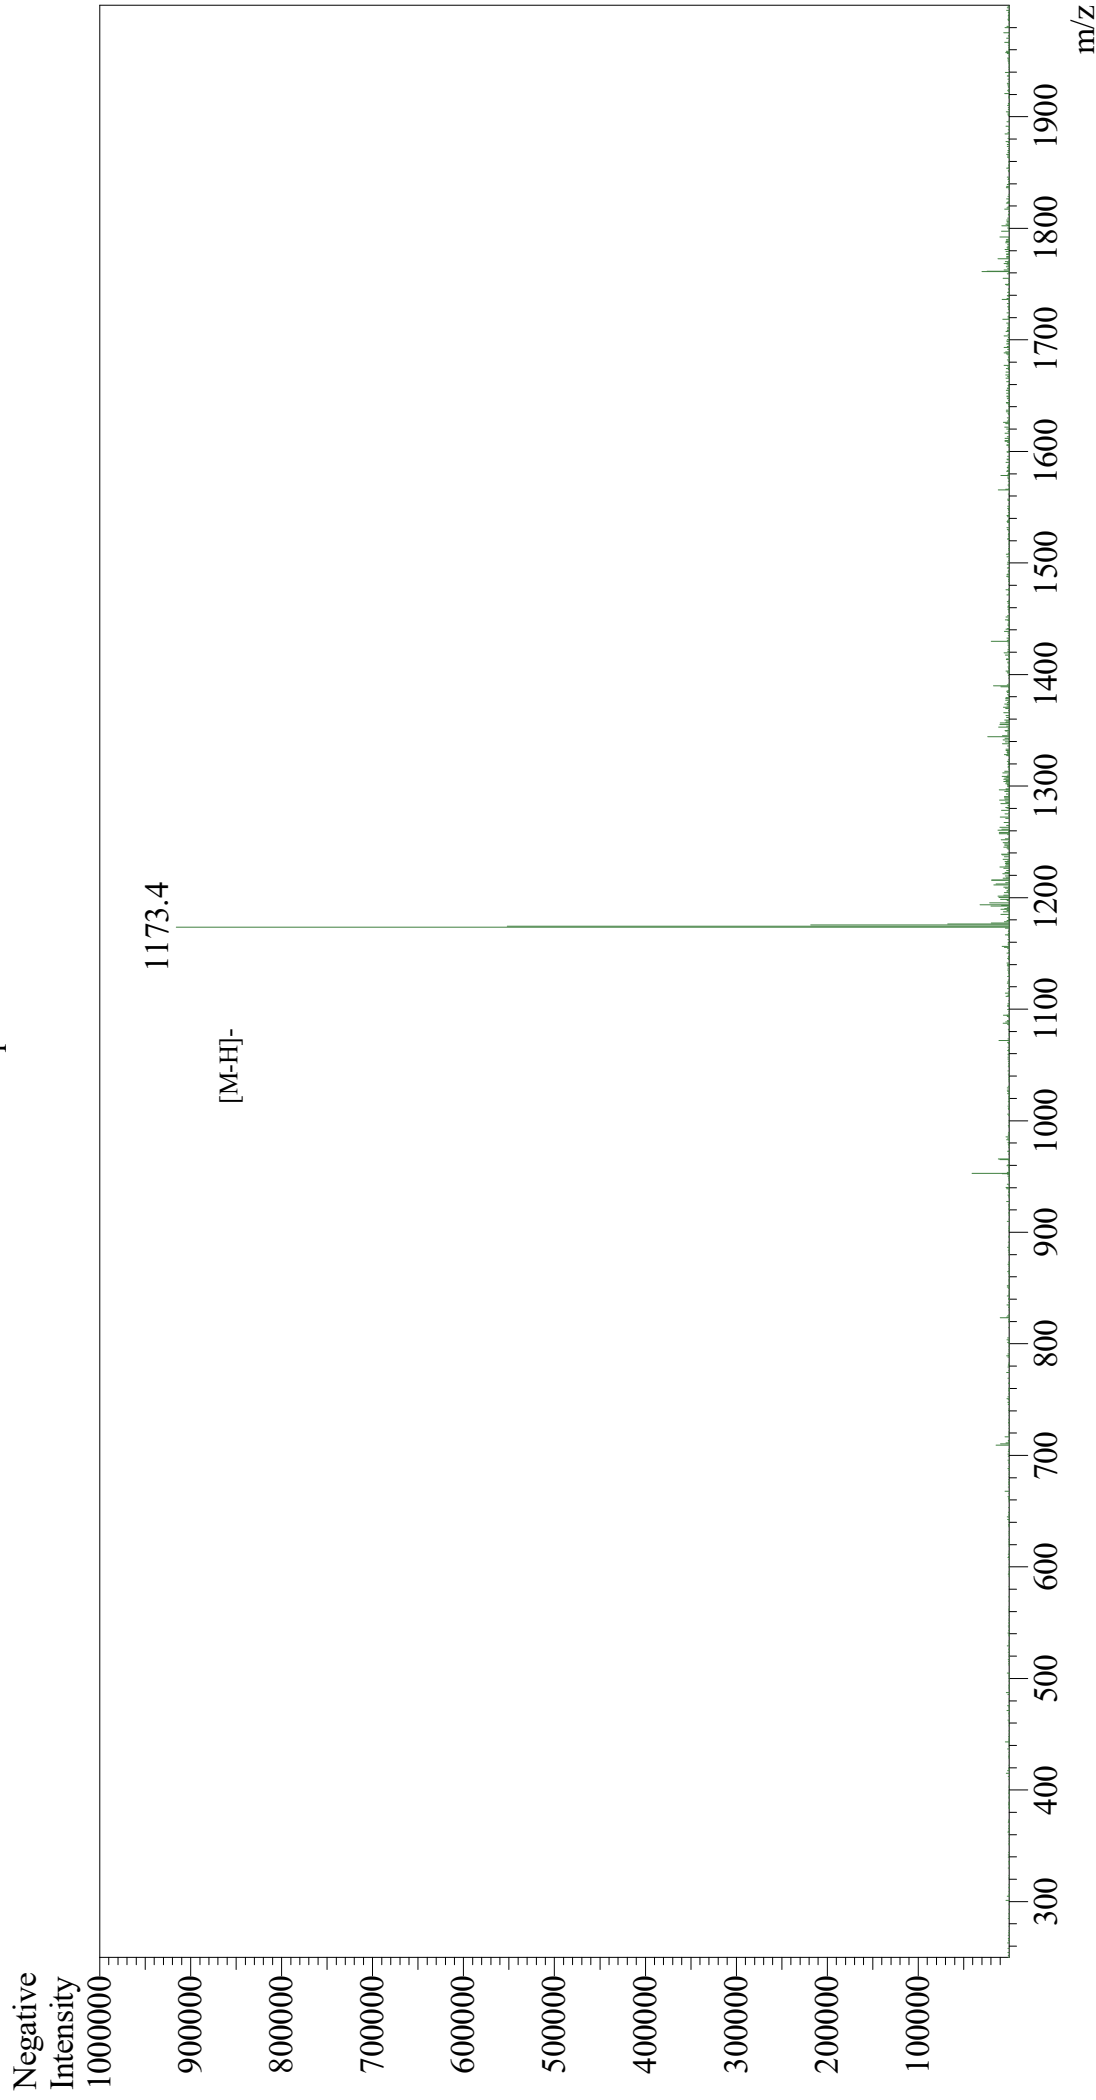

Sample Information
User : Gary
Month-Day Processed : 10/02/19
Time Processed : 05:59:03 PM
Injection Volume : 0.3
Sample Name : mTRP-2(180-188)
Cat No. : RP20250
Lot No. : E7053919J
Theoretical MW : 1175.34
Observed MW : 1174.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : -3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH