

Sample Name : β -Amyloid (25-35)
 Cat No. :RP10008
 Lot No. :PE2441810
 Time Processed:9:52:55
 Month-Day-Year Processed :10/13/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------------|-------|
| 0.01 | Pumps | Pump A B.Conc | 5 |
| 25.00 | Pumps | Pump A B.Conc | 65 |
| 25.01 | Pumps | Pump A B.Conc | 95 |
| 30.00 | Pumps | Pump A B.Conc | 95 |
| 30.01 | Pumps | Pump A B.Conc | 5 |
| 40.00 | Pumps | Pump A B.Conc | 5 |
| 40.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ17010508

<Chromatogram>

mV

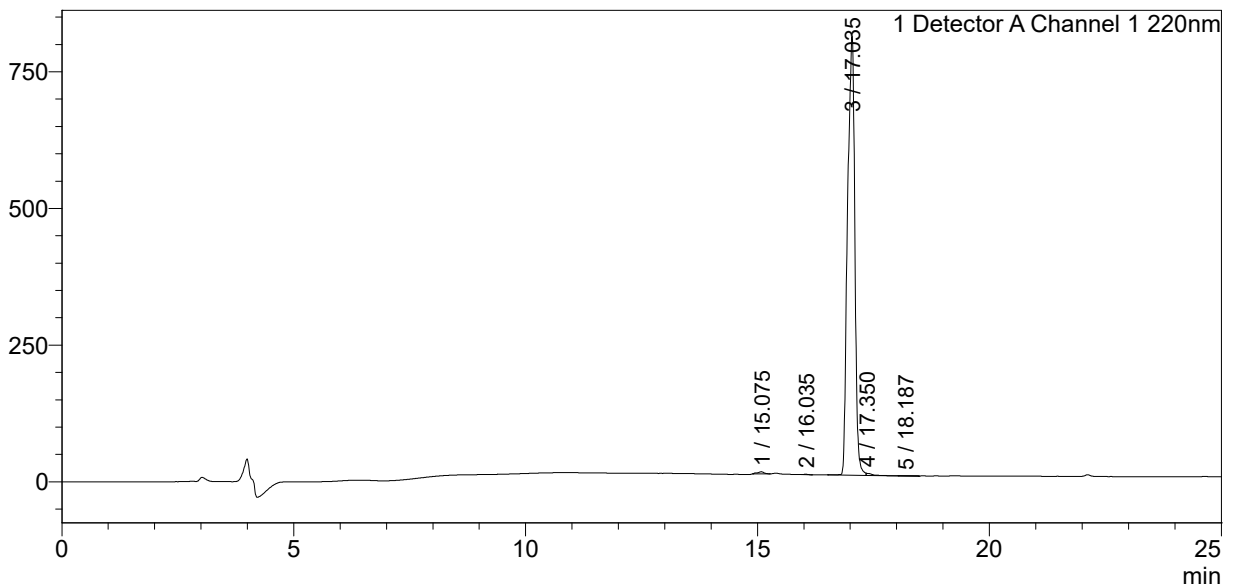

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|--------|---------|
| 1 | 15.075 | 35906 | 3696 | 0.411 |
| 2 | 16.035 | 4869 | 792 | 0.056 |
| 3 | 17.035 | 8671472 | 803401 | 99.187 |
| 4 | 17.350 | 25885 | 3863 | 0.296 |
| 5 | 18.187 | 4379 | 468 | 0.050 |
| Total | | 8742511 | 812221 | 100.000 |