

Sample Name :Osteogenic Growth Peptide, OGP
 Cat No.: RP20311
 Lot No.: E0553020J
 Time Processed :23:01:21
 Month-Day-Year Processed :10/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

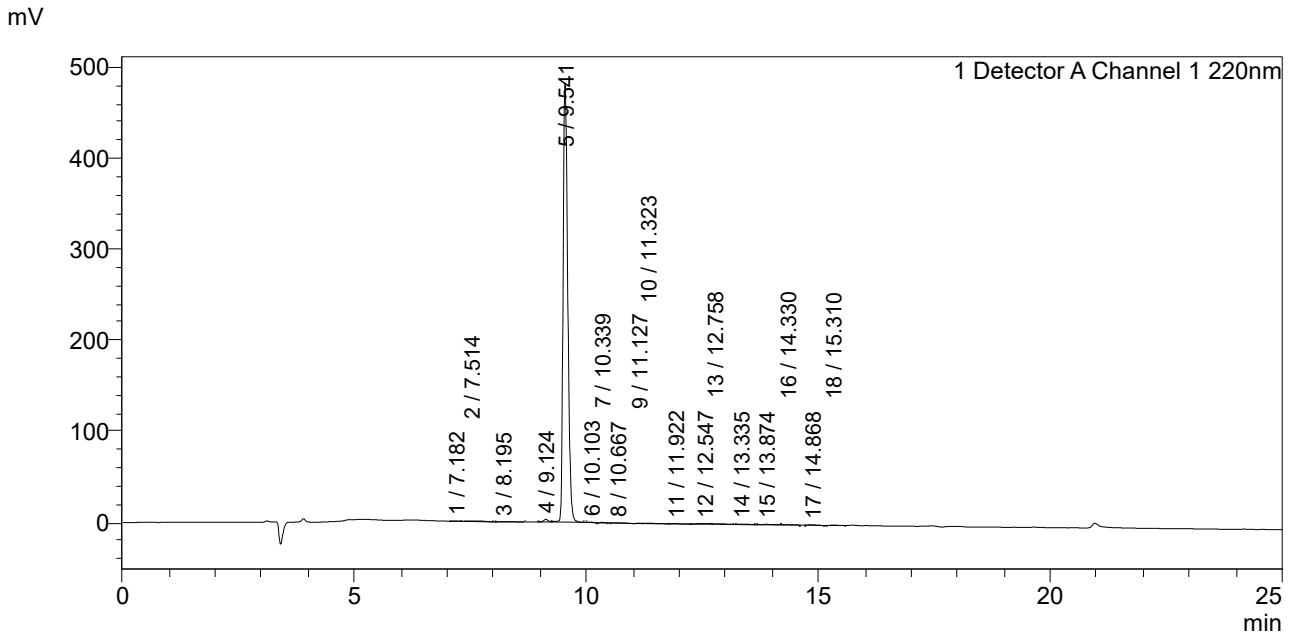

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.182	1191	161	0.034
2	7.514	16297	622	0.471
3	8.195	5826	341	0.169
4	9.124	19010	2790	0.550
5	9.541	3333395	482363	96.423
6	10.103	3837	594	0.111
7	10.339	3688	631	0.107
8	10.667	9168	495	0.265
9	11.127	2894	406	0.084
10	11.323	8988	473	0.260
11	11.922	3460	204	0.100
12	12.547	13544	654	0.392
13	12.758	10114	578	0.293
14	13.335	6618	412	0.191
15	13.874	8133	470	0.235

Peak#	Ret. Time	Area	Height	Area%
16	14.330	3521	313	0.102
17	14.868	4410	343	0.128
18	15.310	2973	222	0.086
Total		3457070	492074	100.000