


Mass Spectrum

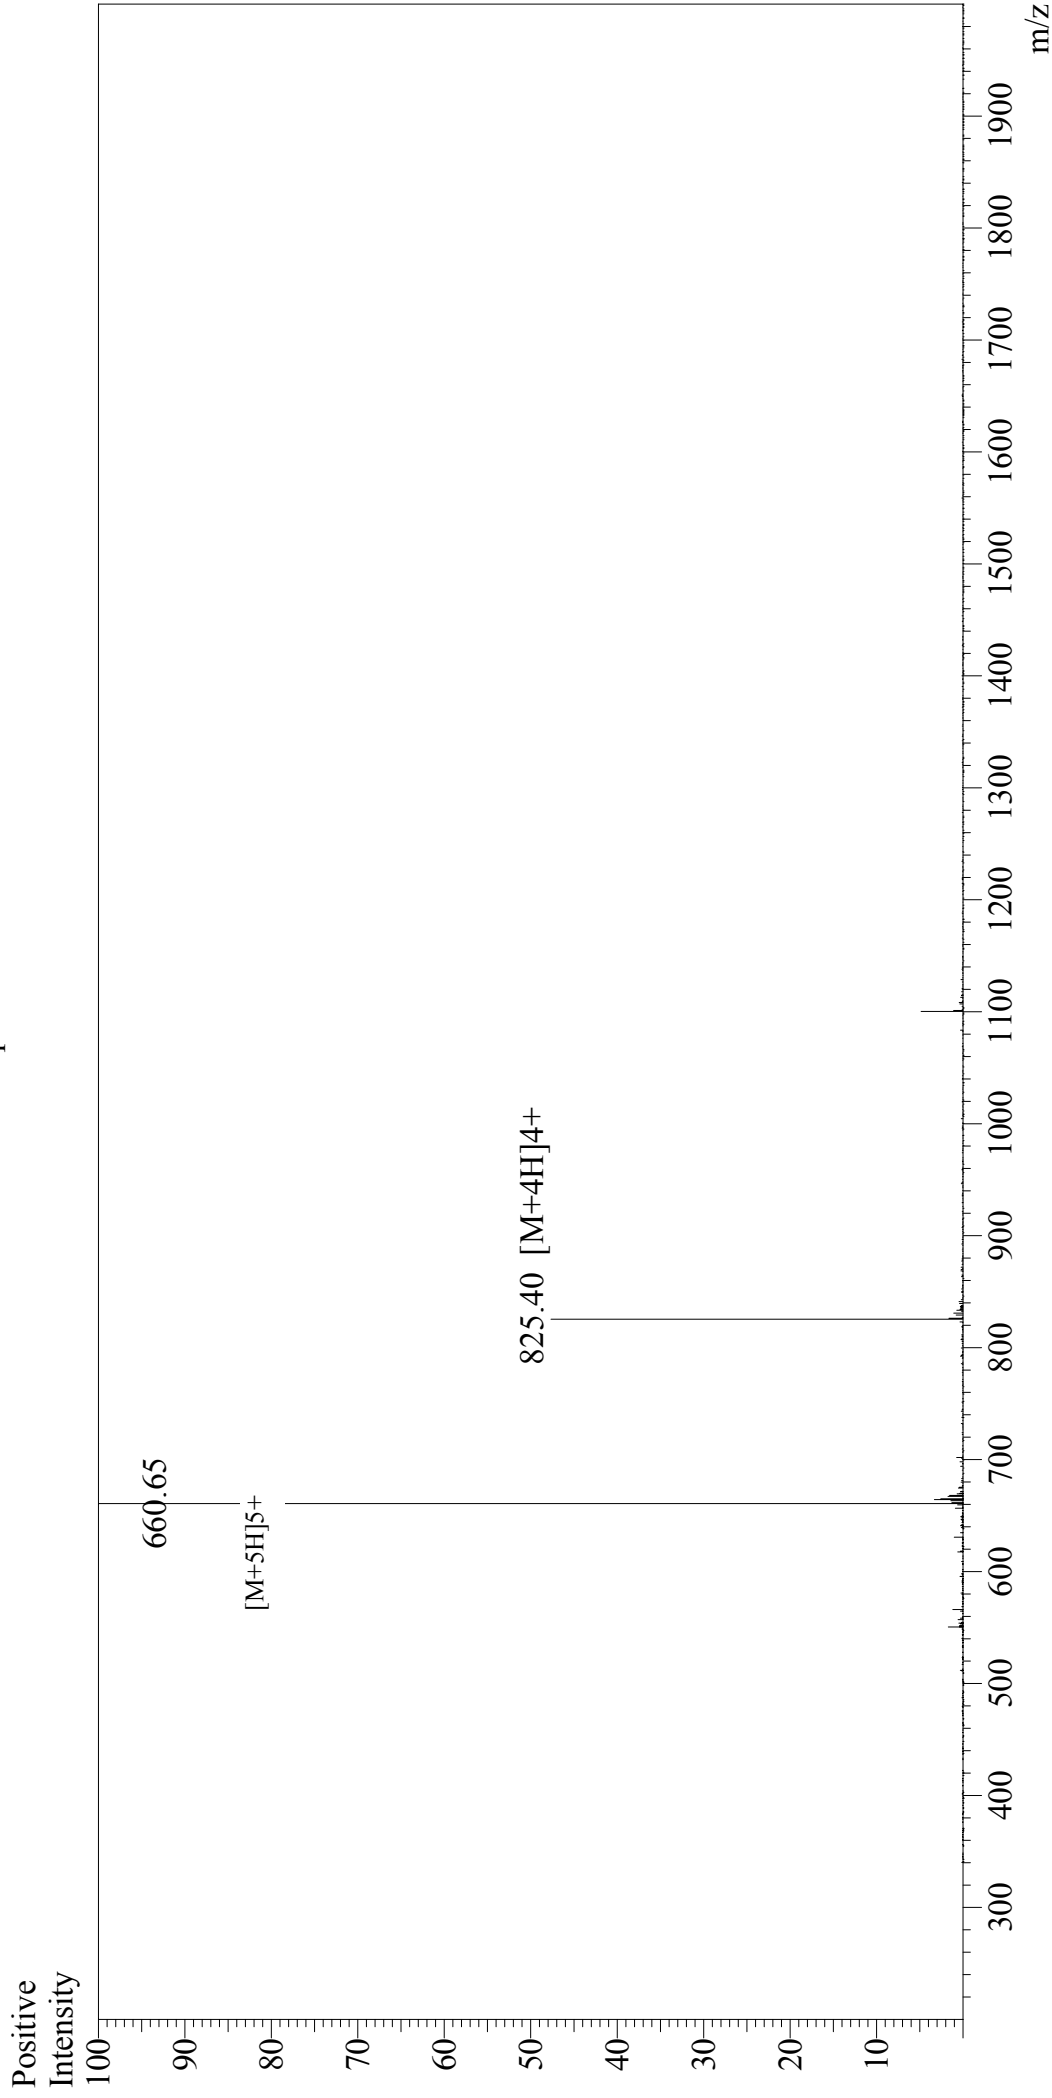

Sample Information

User : Gary
Month-Day Processed : 05/31/18
Time Processed : 18:01:25
Injection Volume : 0.2
Sample Name : GLP-1 (7-36), amide, human
Cat No. : RP10773
Lot No. : PE6061805
Theoretical MW : 3297.65
Observed MW : 3298.25

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH