

Sample Name :Neuropeptide Y, human
 Cat No. :RP10492
 Lot No. :E5715619F
 Time Processed :9:11:02
 Month-Day-Year Processed :06/30/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

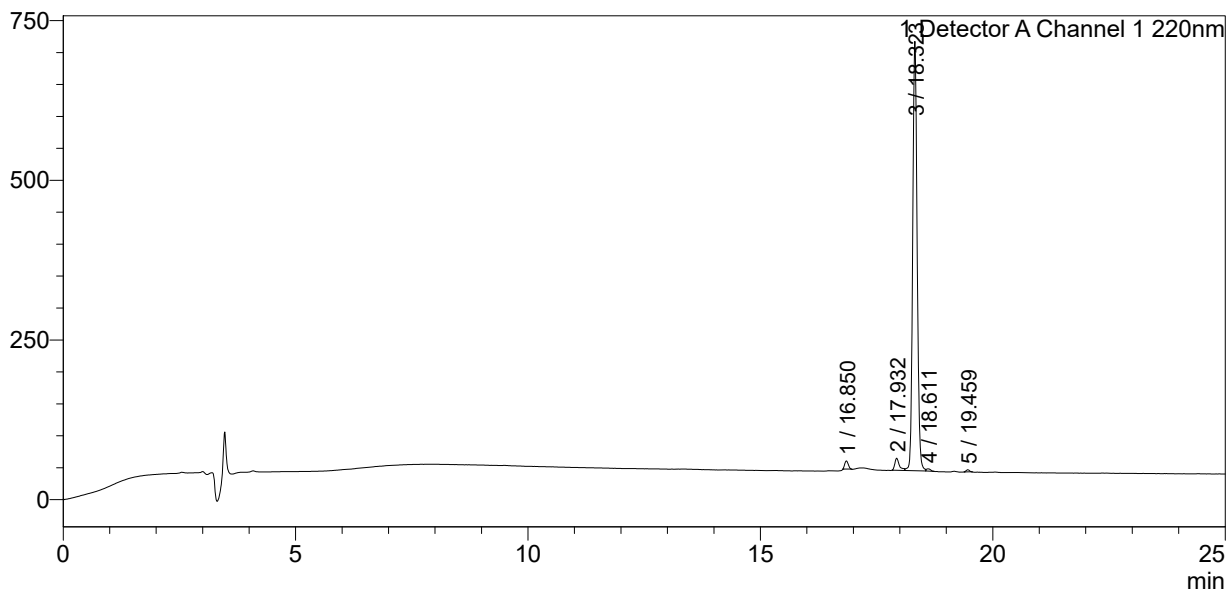

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.850	68029	12842	1.449
2	17.932	128242	18901	2.732
3	18.323	4461061	672120	95.025
4	18.611	20756	3569	0.442
5	19.459	16515	3364	0.352
Total		4694602	710796	100.000