

Sample Name : β -MSH, human
 Cat No. : RP10648
 Lot No. : PE7941902
 Time Processed : 5:58:32
 Month-Day-Year Processed : 03/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK12010012

<Chromatogram>

mV

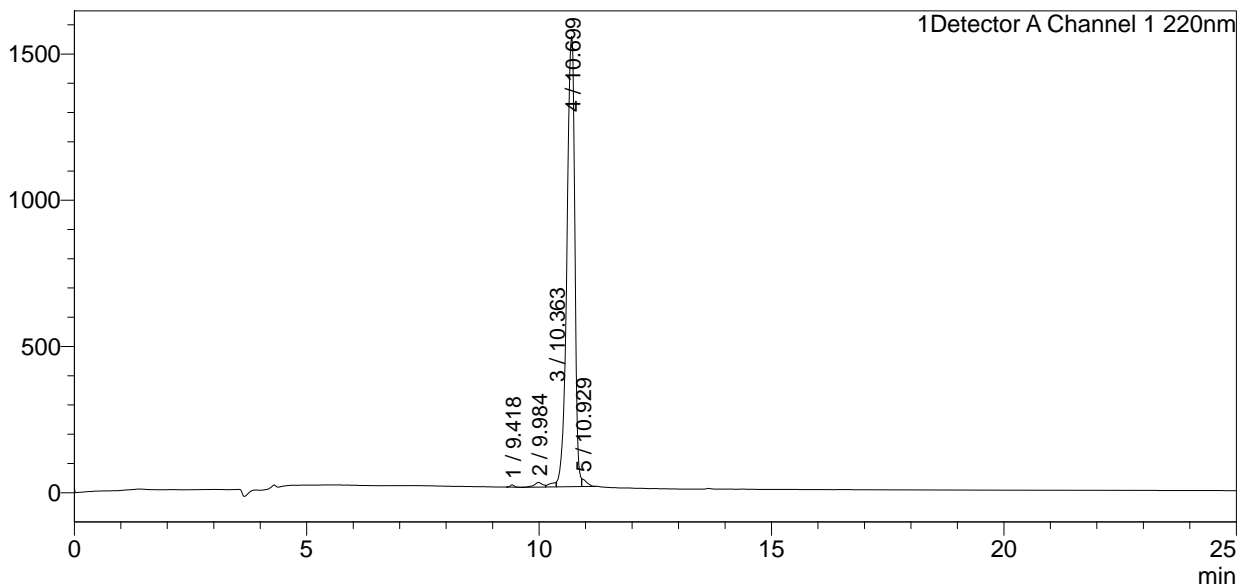

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.418	45574	7639	0.243
2	9.984	198408	15846	1.058
3	10.363	147784	15000	0.788
4	10.699	18176850	1539120	96.951
5	10.929	179900	25826	0.960
Total		18748517	1603431	100.000