

Sample Name : β -Amyloid (33-40)
 Cat No. :RP20144
 Lot No. :E6387819G
 Time Processed :10:57:06 AM
 Month-Day-Year Processed :07/15/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	0
41.00	Pumps	Solvent B Conc.	0
41.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

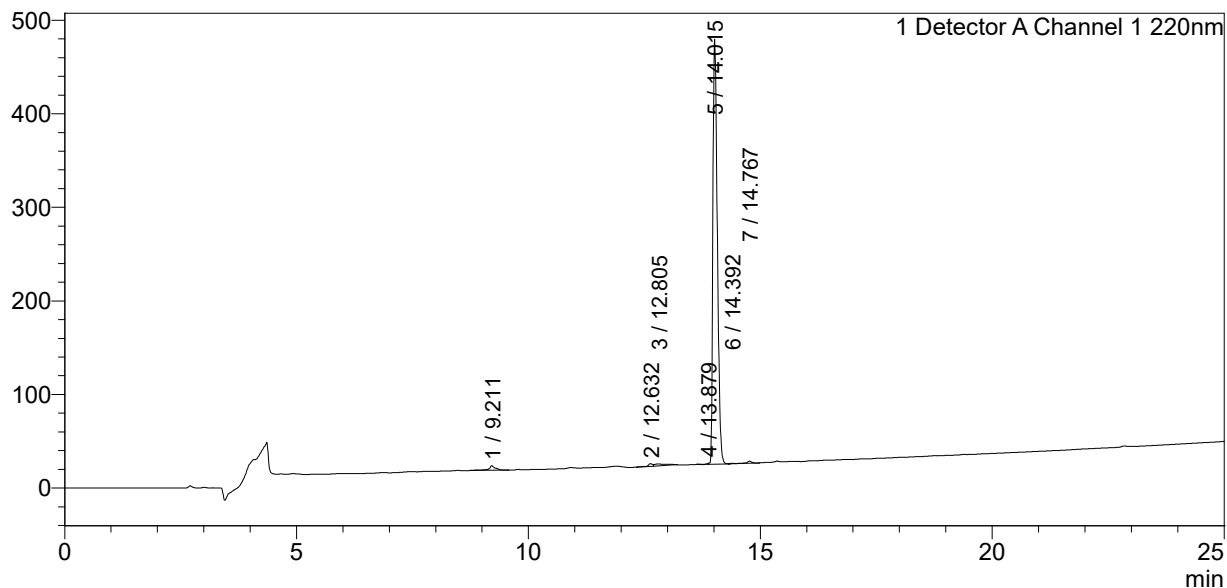

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.211	51366	4924	1.629
2	12.632	18412	2732	0.584
3	12.805	33234	1950	1.054
4	13.879	934	896	0.030
5	14.015	3035278	454303	96.231
6	14.392	2776	554	0.088
7	14.767	12146	2056	0.385
Total		3154145	467413	100.000