

Sample Name :c-Myc Peptide
 Cat. No. :RP11731
 Lot. No. :E0629319H
 Time Processed : 7:53:33
 Month-Day-Year Processed : 08/15/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

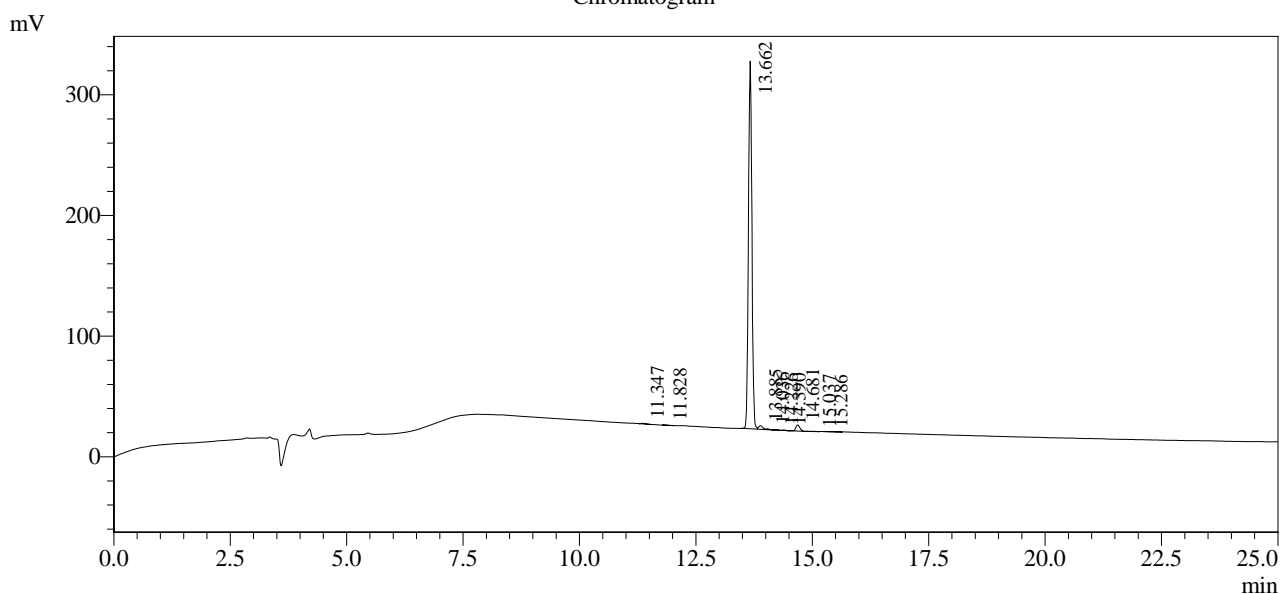

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.347	2824	465	0.174
2	11.828	1376	242	0.085
3	13.662	1561523	304646	96.024
4	13.885	17478	2952	1.075
5	14.036	3542	694	0.218
6	14.226	1924	351	0.118
7	14.390	2522	608	0.155
8	14.681	31640	5111	1.946
9	15.037	1303	162	0.080
10	15.286	2046	193	0.126
Total		1626178	315425	100.000