

Sample Name : HA Peptide  
 Cat No. : RP11735  
 Lot No. : E0631521E  
 Time Processed : 9:11:46  
 Month-Day-Year Processed : 06/03/2021  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
32.00	Pumps	B.Conc	95
32.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
95.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010324

<Chromatogram>

mV

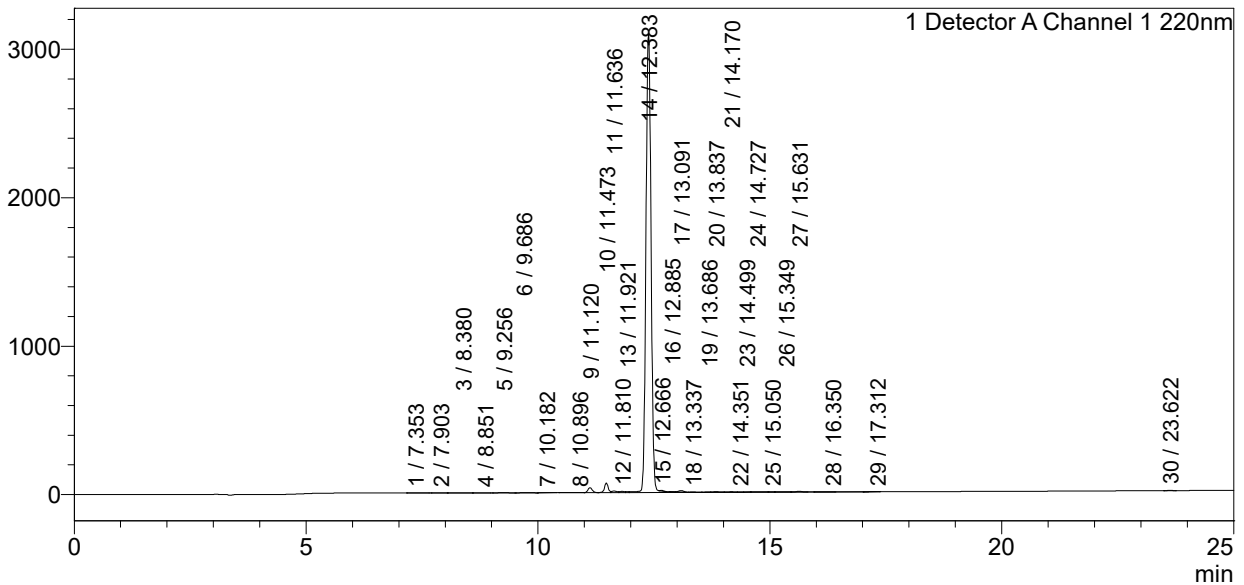

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.353	3750	271	0.015
2	7.903	1157	114	0.005
3	8.380	4516	250	0.018
4	8.851	1611	113	0.006
5	9.256	10404	902	0.042
6	9.686	7468	808	0.030
7	10.182	2796	217	0.011
8	10.896	12740	1346	0.051
9	11.120	218991	33230	0.880
10	11.473	366653	65356	1.474
11	11.636	80711	10103	0.324
12	11.810	58667	7696	0.236
13	11.921	23956	5443	0.096
14	12.383	23809658	3088474	95.723
15	12.666	17344	3981	0.070
16	12.885	5444	1220	0.022

Peak#	Ret. Time	Area	Height	Area%
17	13.091	75911	9680	0.305
18	13.337	10285	1702	0.041
19	13.686	11800	1596	0.047
20	13.837	41736	4491	0.168
21	14.170	28010	2731	0.113
22	14.351	3167	552	0.013
23	14.499	1736	282	0.007
24	14.727	16752	1966	0.067
25	15.050	1430	198	0.006
26	15.349	4118	282	0.017
27	15.631	41225	5374	0.166
28	16.350	1817	51	0.007
29	17.312	2315	92	0.009
30	23.622	7289	1078	0.029
Total		24873459	3249597	100.000