

Sample Name : Calcitonin Gene Related Peptide (CGRP) II, rat
 Cat No. : RP11092
 Lot No. : E6338721A
 Time Processed : 5:46:47
 Month-Day-Year Processed : 02/02/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK12010012

<Chromatogram>

mV

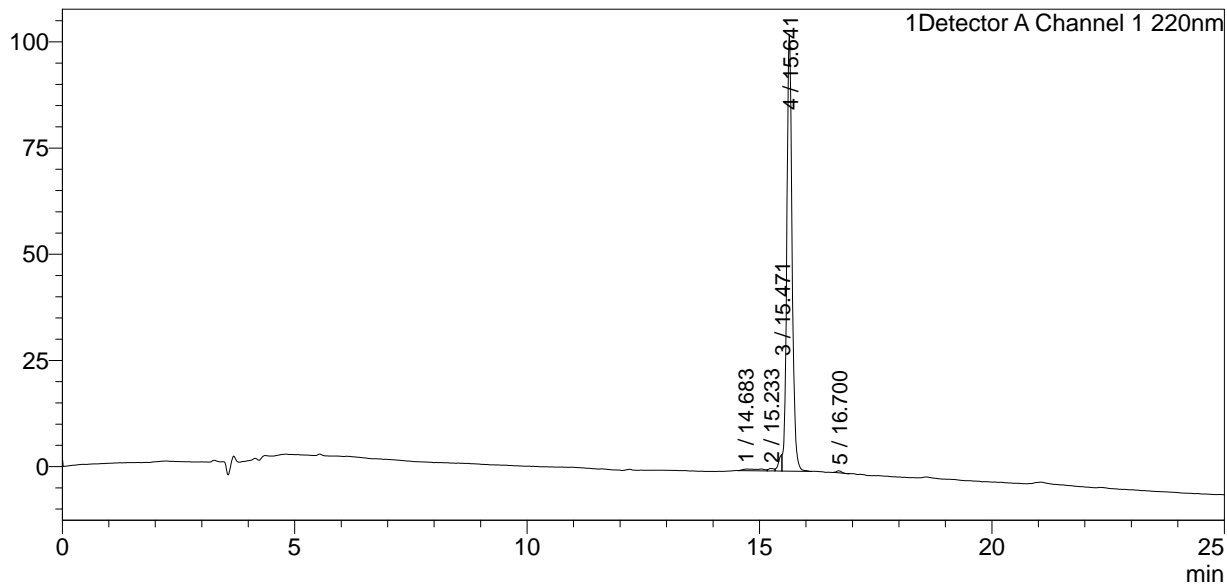

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.683	11440	323	1.344
2	15.233	4841	555	0.569
3	15.471	19595	3714	2.301
4	15.641	812263	101864	95.403
5	16.700	3260	465	0.383
Total		851399	106920	100.000