

Sample Name : Apidaecin IB
 Cat. No. : RP20409
 Lot. No. : E2862620B
 Time Processed : 20:05:00
 Month-Day-Year Processed : 02/29/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

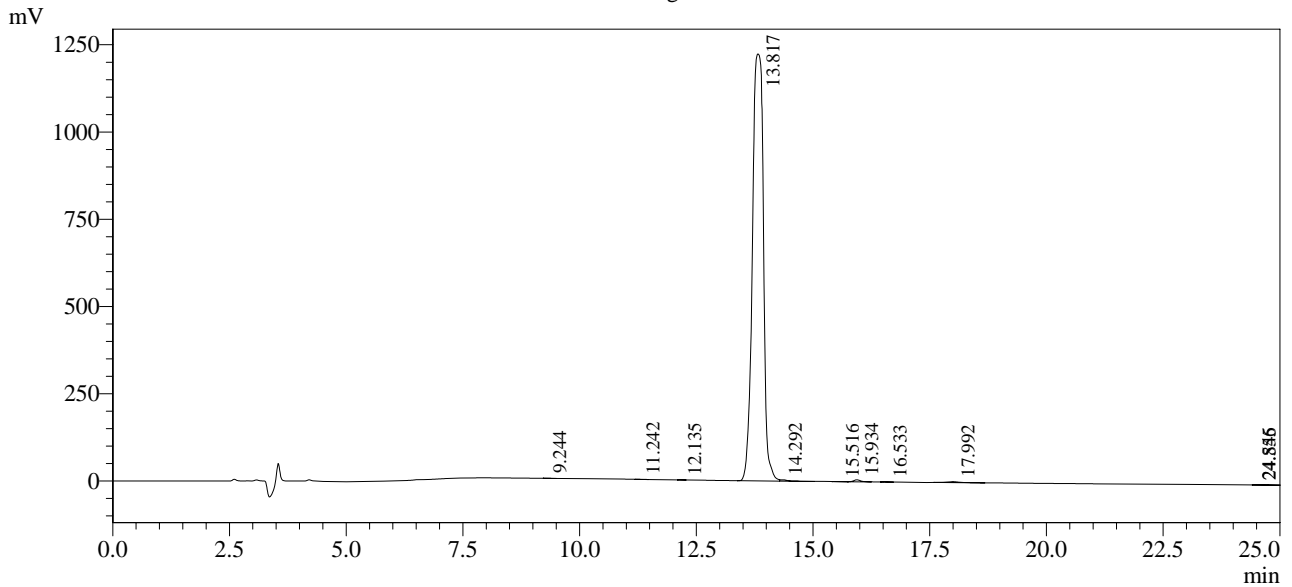

1 Det. A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.244	1819	176	0.009
2	11.242	1718	268	0.009
3	12.135	1084	216	0.005
4	13.817	20020324	1223365	99.092
5	14.292	50308	3884	0.249
6	15.516	3320	396	0.016
7	15.934	57685	5609	0.286
8	16.533	2367	435	0.012
9	17.992	56682	2826	0.281
10	24.546	6519	868	0.032
11	24.855	2018	227	0.010
Total		20203842	1238269	100.000