

Sample Name : HA Peptide
 Cat. No. : RP11735
 Lot. No. : E7126921C
 Time Processed : 2:24:30 PM
 Month-Day-Year Processed : 03/27/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------------|-------|
| 0.01 | Pumps | Pump A B.Conc | 5 |
| 25.00 | Pumps | Pump A B.Conc | 65 |
| 25.01 | Pumps | Pump A B.Conc | 95 |
| 27.00 | Pumps | Pump A B.Conc | 95 |
| 27.01 | Pumps | Pump A B.Conc | 5 |
| 35.00 | Pumps | Pump A B.Conc | 5 |
| 35.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : GK11010011

<Chromatogram>

mV

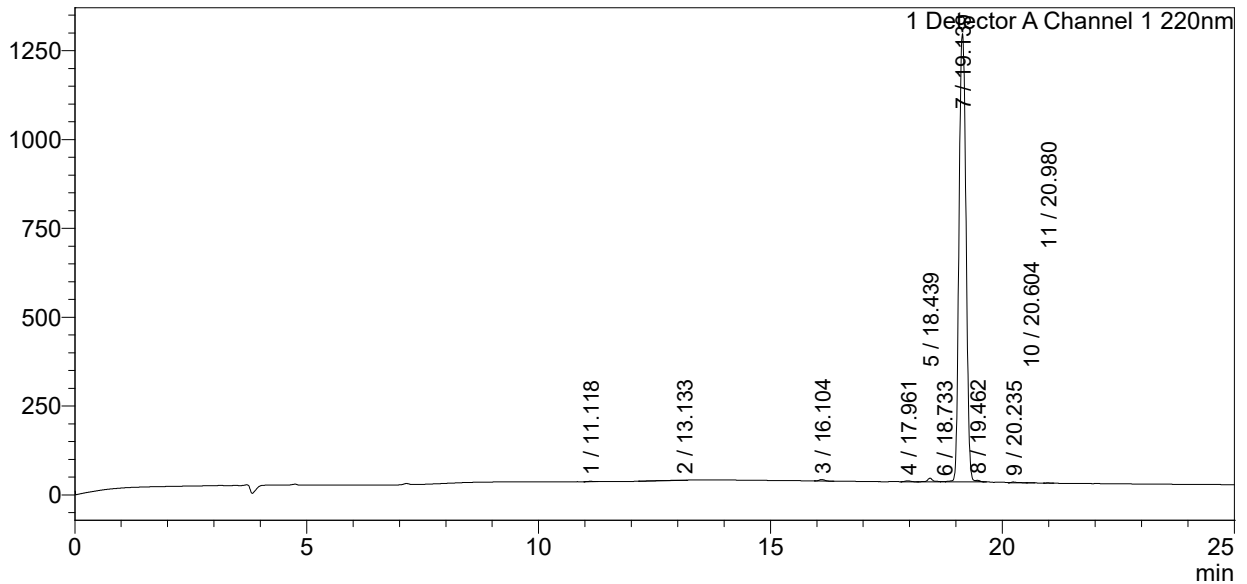

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|----------|---------|---------|
| 1 | 11.118 | 8150 | 1169 | 0.061 |
| 2 | 13.133 | 16213 | 143 | 0.121 |
| 3 | 16.104 | 35760 | 4399 | 0.267 |
| 4 | 17.961 | 24992 | 2909 | 0.186 |
| 5 | 18.439 | 90919 | 10631 | 0.678 |
| 6 | 18.733 | 9079 | 1465 | 0.068 |
| 7 | 19.139 | 13181312 | 1262299 | 98.350 |
| 8 | 19.462 | 9596 | 1882 | 0.072 |
| 9 | 20.235 | 18847 | 2125 | 0.141 |
| 10 | 20.604 | 2611 | 575 | 0.019 |
| 11 | 20.980 | 4968 | 911 | 0.037 |
| Total | | 13402448 | 1288508 | 100.000 |